

Sample Name :Flagelin22  
 Cat. No. : RP19986  
 Lot. No. : E1827319L  
 Time Processed : 12:37:45  
 Month-Day-Year Processed : 12/26/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
 Total Flow:1 ml/min  
 Wavelength:220 nm

Time	Unit	Command	Value	Comment
0.01	Pumps	Pump A B.Conc	5	
25.00	Pumps	Pump A B.Conc	65	
25.01	Pumps	Pump A B.Conc	95	
27.00	Pumps	Pump A B.Conc	95	
27.01	Pumps	Pump A B.Conc	5	
35.00	Pumps	Pump A B.Conc	5	
35.01	Controller	Stop		


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

Equipment: GK11010011

Chromatogram

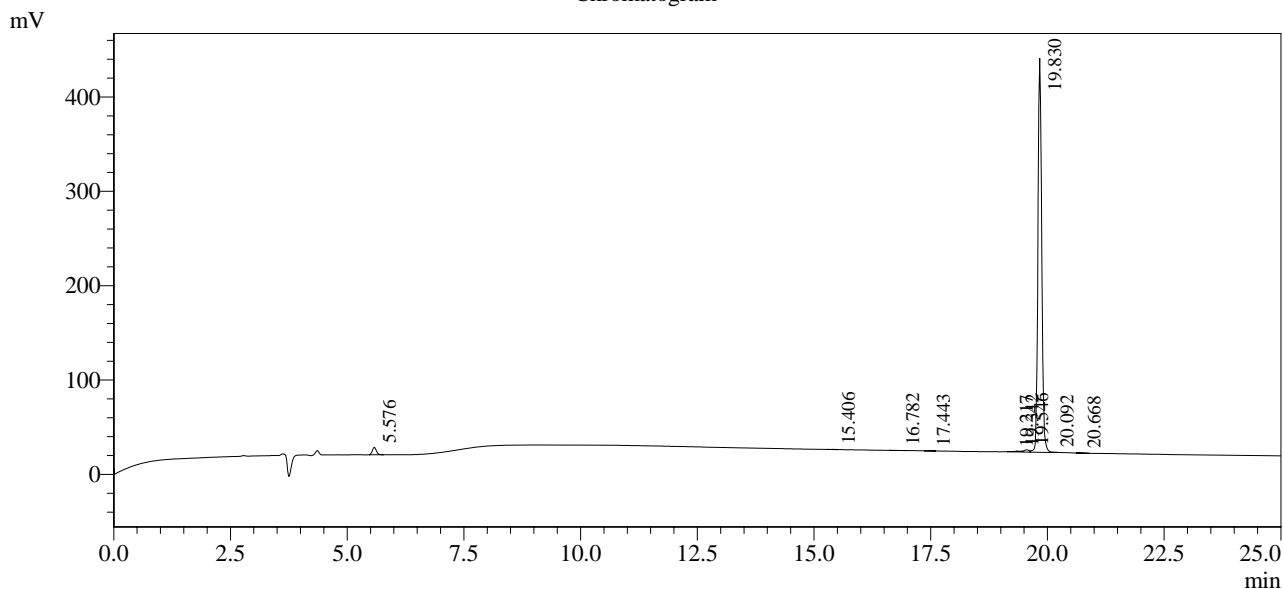

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	5.576	46592	7807	1.899
2	15.406	682	137	0.028
3	16.782	2409	318	0.098
4	17.443	517	108	0.021
5	19.217	1560	303	0.064
6	19.342	8475	827	0.345
7	19.546	18090	2459	0.737
8	19.830	2371998	417556	96.673
9	20.092	2145	422	0.087
10	20.668	1163	127	0.047
Total		2453631	430064	100.000