

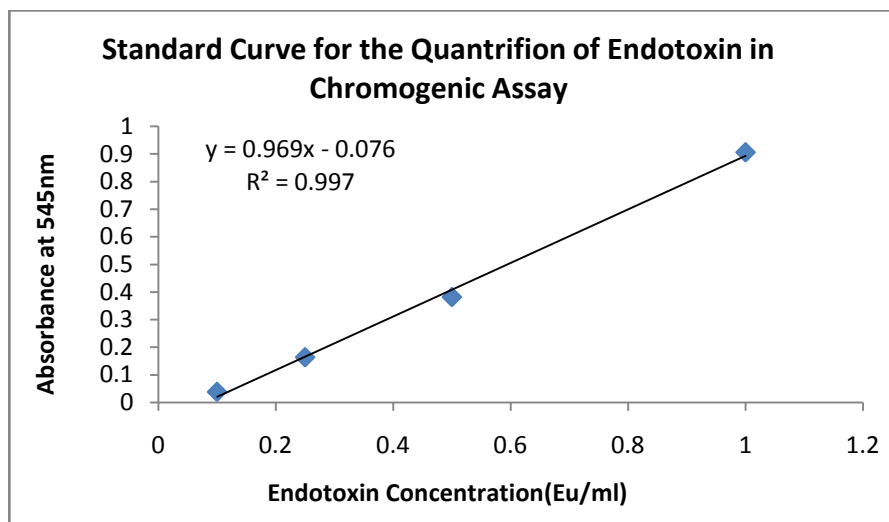
## CERTIFICATE OF ANALYSIS

**Product Information**

Product Name:	ToxinSensor™ Chromogenic LAL Endotoxin Assay Kit
Cat. No.:	L00350
Lot No.:	C50091512
Exp.Date:	01 Jun 2017

**Kit Contents**

Kit Components	Lot.No	Storage Condition
LAL Reagent Water	C50081512	Store at 2-8°C
Limulus Amebocyte Lysate (LAL)	C50011512	Store at 2-8°C
<i>E. coli</i> Endotoxin Standard	C50021512	Store at 2-8°C
Chromogenic Substrate	C50031512	Store at 2-8°C
Buffer S for Color-stabilizer #1	C50071512	Store at 2-8°C
Color-stabilizer #1	C50041512	Store at 2-8°C
Color-stabilizer #2	C50051512	Store at 2-8°C
Color-stabilizer #3	C50061512	Store at 2-8°C
Endotoxin-free tubes	C50291512	Store at 2-8°C
Endotoxin-free Tips, 200 µl	---	Store at 2-8°C
Endotoxin-free Tips, 1000 µl	C50301501	Store at 2-8°C
Incubation Rack	---	Store at 2-8°C

**Endpoint Chromogenic LAL Assay**


---

<b>Test</b>		<b>Results</b>
Sensitivity (OD 545nm)	Blank	0.055
	Maxi Endotoxin Standards	0.960
Linearity	Correlation Coefficient (R <sup>2</sup> )	0.997
	Endotoxin-free Tips, 1000 µl	0.005
Endotoxin-free materials (EU/ml)	Endotoxin-free tubes	0.004

---

**Caution:**

For laboratory or further manufacturing use only. Not intended for household use. If you have any questions about the Certificate of Analysis, please contact our customer service representative at 1-877-436-7274 (Toll-Free), or 1-732-885-9188.

Certified by: *Neo Li* Date: 07/01/2015  
Product Department