

## CERTIFICATE OF ANALYSIS


### Product Information

Product Name:	ToxinSensor™ Chromogenic LAL Endotoxin Assay Kit
Cat. No.:	L00350
Lot No.:	C50091710
Exp.Date:	01 Aug 2019

### Kit Contents

Kit Components	Lot.No	Storage Condition
LAL Reagent Water	C50081710	Store at 2-8°C
Limulus Amebocyte Lysate (LAL)	C50011710	Store at 2-8°C
<i>E. coli</i> Endotoxin Standard	C50021710	Store at 2-8°C
Chromogenic Substrate	C50031710	Store at 2-8°C
Buffer S for Color-stabilizer #1	C50071710	Store at 2-8°C
Color-stabilizer #1	C50041710	Store at 2-8°C
Color-stabilizer #2	C50051710	Store at 2-8°C
Color-stabilizer #3	C50061710	Store at 2-8°C
Endotoxin-free tubes	C50291704	Store at 2-8°C
Endotoxin-free Tips, 200 µl	---	Store at 2-8°C
Endotoxin-free Tips, 1000 µl	C50301704	Store at 2-8°C
Incubation Rack	---	Store at 2-8°C

### Endpoint Chromogenic LAL Assay

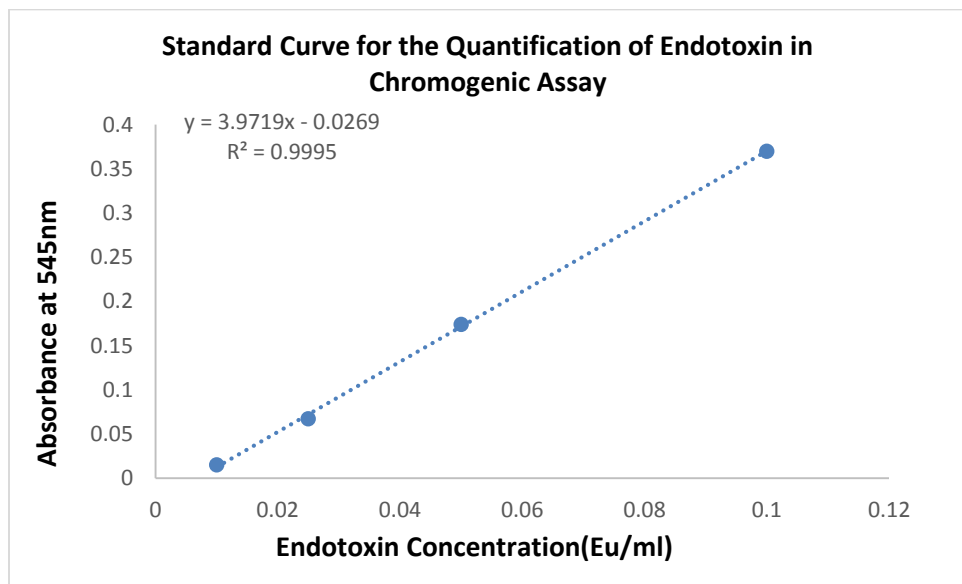

---

<b>Test</b>		<b>Results</b>
Sensitivity (OD 545nm)	Blank	0.061
	Maxi Endotoxin Standards	0.431
Linearity	Correlation Coefficient (R <sup>2</sup> )	0.9995
	Endotoxin-free Tips, 1000 µl	0.005
Endotoxin-free materials (EU/ml)	Endotoxin-free tubes	0.004

---

**Caution:**

For laboratory or further manufacturing use only. Not intended for household use. If you have any questions about the Certificate of Analysis, please contact our customer service representative at 1-877-436-7274 (Toll-Free), or 1-732-885-9188.

Certified by: *Neo Li* Date: 09/01/2017  
Product Department