

Sample Name : $\beta$ -Amyloid (42-1)  
 Cat No.: RP10034  
 Lot No. : PE8191902  
 Time Processed : 9:20:14  
 Month-Day-Year Processed : 03/08/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
 Total Flow: 1 ml/min  
 Wavelength: 220 nm

Time	Unit	Command	Value	Comment
0.01	Pumps	Pump B Conc.	15	
25.00	Pumps	Pump B Conc.	75	
25.01	Pumps	Pump B Conc.	95	
31.00	Pumps	Pump B Conc.	95	
31.01	Pumps	Pump B Conc.	15	
37.00	Pumps	Pump B Conc.	15	
37.01	Controller	Stop		


<<Column Performance>>

<Detector A>

Column : UniPS 10-300 4.6 x 250 mm

Equipment: GR09010180

Chromatogram

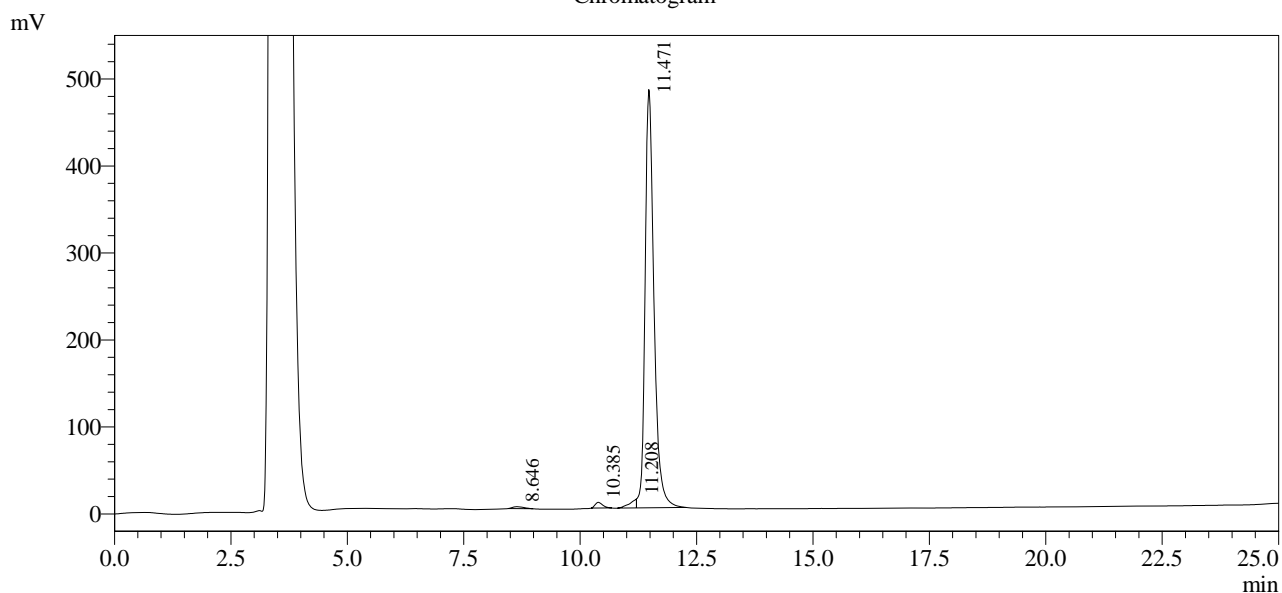

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	8.646	36097	2182	0.548
2	10.385	72548	6479	1.101
3	11.208	100605	10218	1.526
4	11.471	6382754	480838	96.826
Total		6592004	499716	100.000