

Sample Name :Flagelin22  
 Cat No :RP19986  
 Lot No :E4575521A  
 Time Processed :1:44:45  
 Month-Day-Year Processed :01/20/2021


Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
 Total Flow:1 ml/min  
 Wavelength:220 nm

Time	Module	Command	Value
0.01	Pumps	Pump A B.Conc	5
25.00	Pumps	Pump A B.Conc	65
25.01	Pumps	Pump A B.Conc	95
27.00	Pumps	Pump A B.Conc	95
27.01	Pumps	Pump A B.Conc	5
35.00	Pumps	Pump A B.Conc	5
35.01	Controller	Stop	

<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

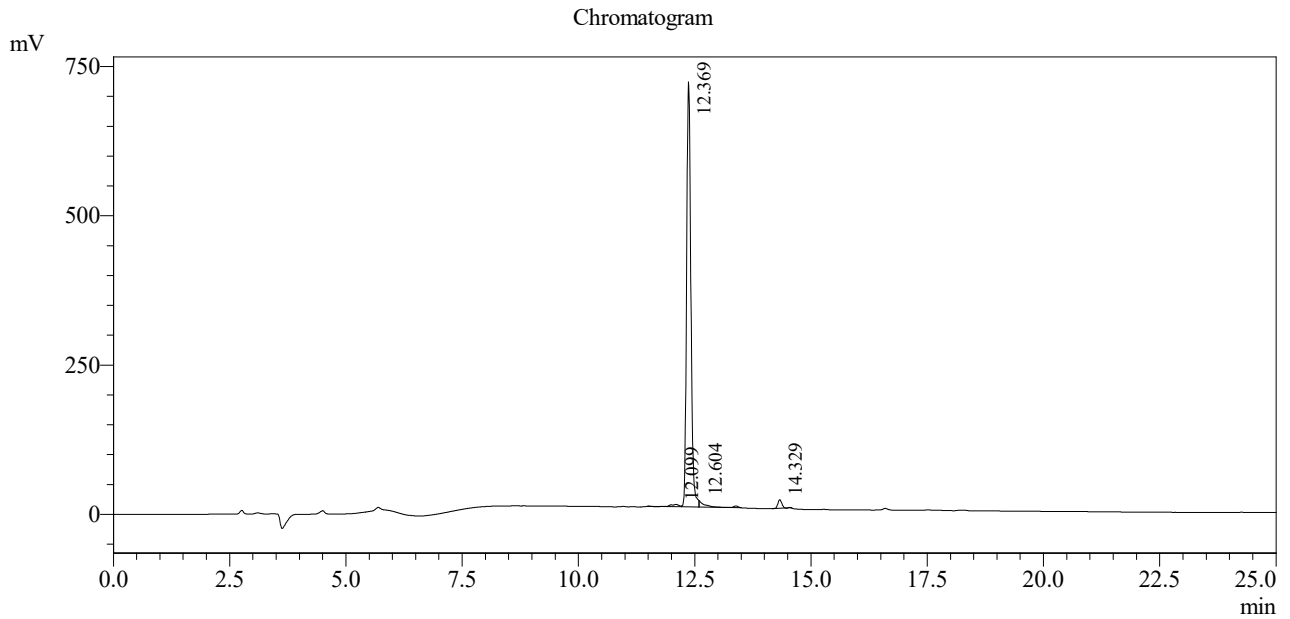

Peak Table

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	12.099	42832	3846	0.904
2	12.369	4516197	711693	95.355
3	12.604	94626	10310	1.998
4	14.329	82562	14181	1.743
Total		4736217	740031	100.000