

Sample Name :Flagelin22
 Cat No :RP19986
 Lot No :E8165320L
 Time Processed :13:08:32
 Month-Day-Year Processed :12/23/2020


Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

Time	Module	Command	Value
0.01	Pumps	B.Conc	5
25.00	Pumps	B.Conc	65
25.01	Pumps	B.Conc	95
30.00	Pumps	B.Conc	95
35.00	Pumps	B.Conc	5
62.00	Pumps	B.Conc	5
70.00	Controller	Stop	

<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

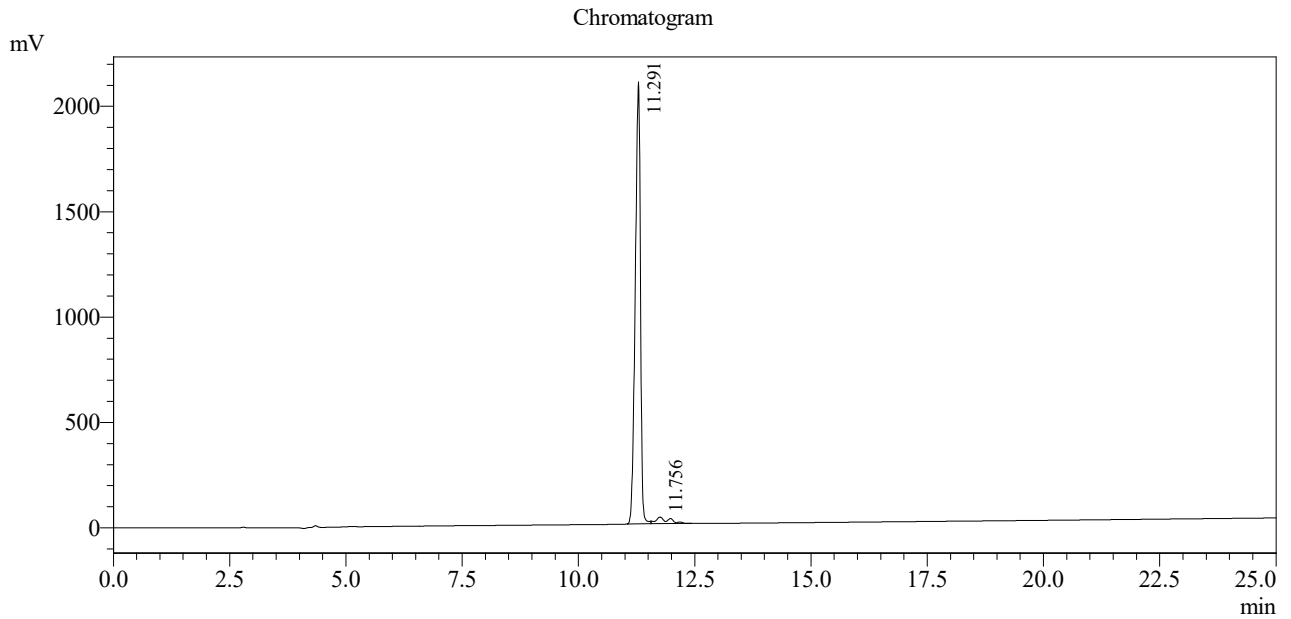

1 Detector A Channel 1 / 220nm

Peak Table

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	11.291	16212770	2096744	96.324
2	11.756	618789	31273	3.676
Total		16831559	2128017	100.000