

Sample Information

Sample Name :Urocortin II, human
 Cat. No :RP10098
 Lot. No. :PE6841710

Pump A : 0.065% trifluoroacetic in 100% waters (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)


<<Pump>>
 Flow : 1.0000 mL/min

<<Detector A>>
 Wavelength Ch1 : 220 nm

<<LC Time Program>>

Time	Module	Command	Value	Comment
0.01	Pumps	Solvent B Conc.	5	
10.00	Pumps	Solvent B Conc.	35	
35.00	Pumps	Solvent B Conc.	95	
37.00	Pumps	Solvent B Conc.	95	
37.01	Pumps	Solvent B Conc.	5	
45.00	Pumps	Solvent B Conc.	5	
45.01	Controller	Stop		

<<Column Performance>>
 <Detector A>
 Column : Inertsil ODS-3 4.6 x 250 mm

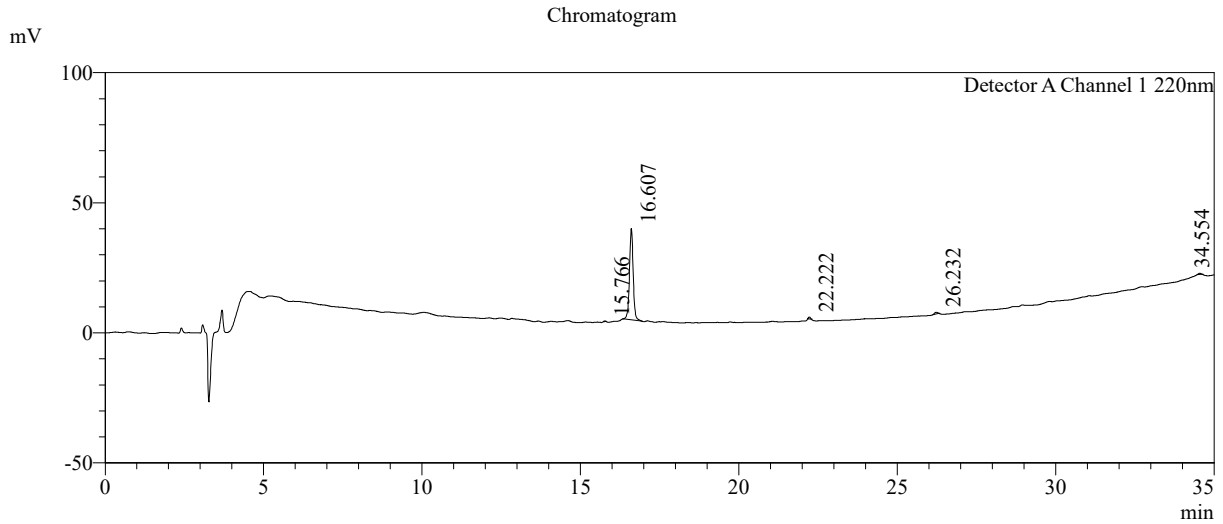

Peak Table

Peak#	Ret. Time	Height	Area	Height%	Area%
1	15.766	179	447	0.483	0.152
2	16.607	35105	284152	94.777	96.543
3	22.222	698	2784	1.884	0.946
4	26.232	594	4086	1.603	1.388
5	34.554	464	2859	1.253	0.971
Total		37040	294328	100.000	100.000