

Sample Name : β -Amyloid (42-1)
 Cat.No : RP10034
 Lot.No : E9534821B
 Time Processed: 11:15:15
 Year-Month-Day: 2021/4/1

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow: 1 ml/min

<<Detector A>>
 Wavelength Ch1 : 220 nm

<<LC Time Program>>


Time	Module	Command	Value	Comment
0.01	Pumps	Solvent B Conc.	5	
25.00	Pumps	Solvent B Conc.	65	
25.01	Pumps	Solvent B Conc.	95	
27.00	Pumps	Solvent B Conc.	95	
27.01	Pumps	Solvent B Conc.	5	
33.00	Pumps	Solvent B Conc.	5	
33.01	Controller	Stop		

<<Column Performance>>

<Detector A>
 Column : Inertsil ODS-3 4.6 x 250 mm
 Equipment: ZJ19010015

<Chromatogram>

mV

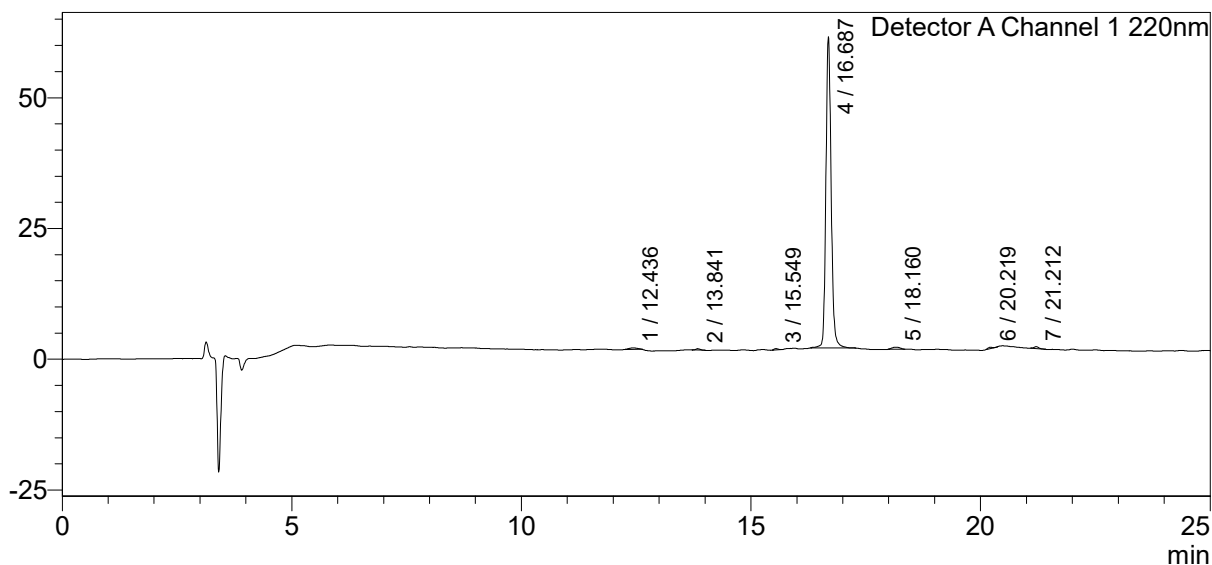

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	12.436	3637	272	0.745
2	13.841	1770	249	0.363
3	15.549	1624	249	0.333
4	16.687	472632	58545	96.826
5	18.160	4422	370	0.906
6	20.219	1664	237	0.341
7	21.212	2375	344	0.487
Total		488124	60265	100.000