

Sample Name :  $\beta$ -Amyloid (1-42), human  
 Cat. No. : RP10017  
 Lot. No. : PE5431809  
 Time Processed : 14:56:05  
 Month-Day-Year Processed : 11/06/2018

Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
 Total Flow: 1 ml/min  
 Wavelength: 220 nm

Time	Unit	Command	Value	Comment
0.01	Pumps	Pump B Conc.	10	
25.00	Pumps	Pump B Conc.	100	
25.01	Pumps	Pump B Conc.	95	
31.00	Pumps	Pump B Conc.	95	
31.01	Pumps	Pump B Conc.	10	
40.00	Pumps	Pump B Conc.	10	
40.01	Controller	Stop		


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

Equipment : SS-CM-0310

Chromatogram

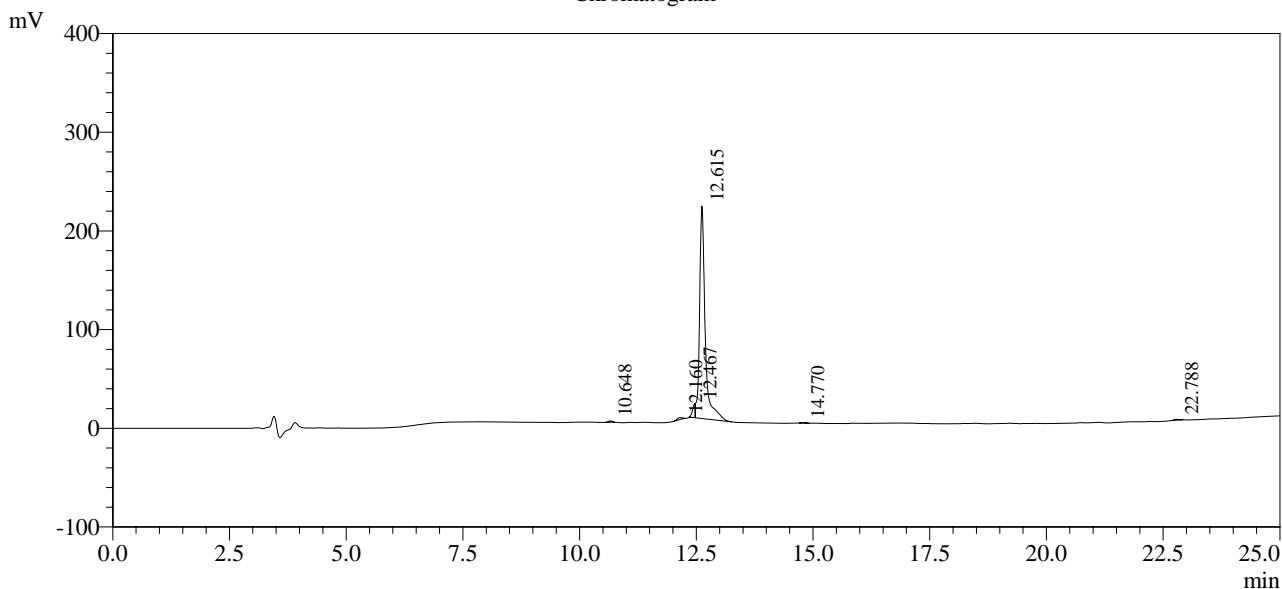

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	10.648	7125	1349	0.376
2	12.160	15787	2099	0.834
3	12.467	55018	14394	2.907
4	12.615	1803649	215328	95.299
5	14.770	2658	449	0.140
6	22.788	8394	1125	0.444
Total		1892630	234744	100.000