

Sample Name : -Amyloid (42-1)
 Cat No. :RP10034
 Lot No. :E0920321H
 Time Processed :4:14:32 PM
 Month-Day-Year Processed :09/28/2021

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	B.Conc	5
25.00	Pumps	B.Conc	65
25.01	Pumps	B.Conc	95
27.00	Pumps	B.Conc	95
27.01	Pumps	B.Conc	5
35.00	Pumps	B.Conc	5
35.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column :Inertsil ODS-3 4.6 x 250 mm
 Equipment: GK11010011

<Chromatogram>

mV

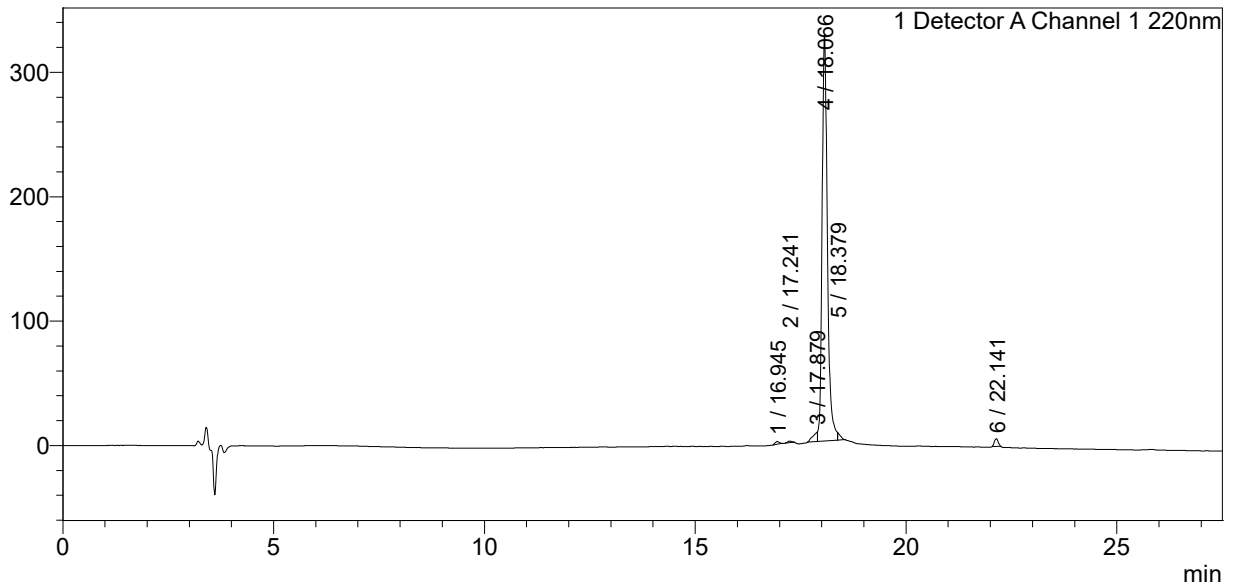

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	16.945	13972	2073	0.466
2	17.241	8340	1209	0.278
3	17.879	59314	6860	1.978
4	18.066	2852429	324625	95.146
5	18.379	25759	6420	0.859
6	22.141	38124	6144	1.272
Total		2997937	347331	100.000