

Sample Name :β-Amyloid (42-1)  
 Cat. No. : RP10034  
 Lot. No. : E5697419F  
 Time Processed :16:11:01  
 Month-Day-Year Processed :08/16/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
 Total Flow:1 ml/min  
 Wavelength:220 nm


Time	Unit	Command	Value	Comment
0.01	Pumps	Pump B Conc.	15	
25.00	Pumps	Pump B Conc.	75	
25.01	Pumps	Pump B Conc.	95	
31.00	Pumps	Pump B Conc.	95	
31.01	Pumps	Pump B Conc.	15	
37.00	Pumps	Pump B Conc.	15	
37.00	Controller	Stop		

<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm  
 Equipment :SS-CM-0310

Chromatogram

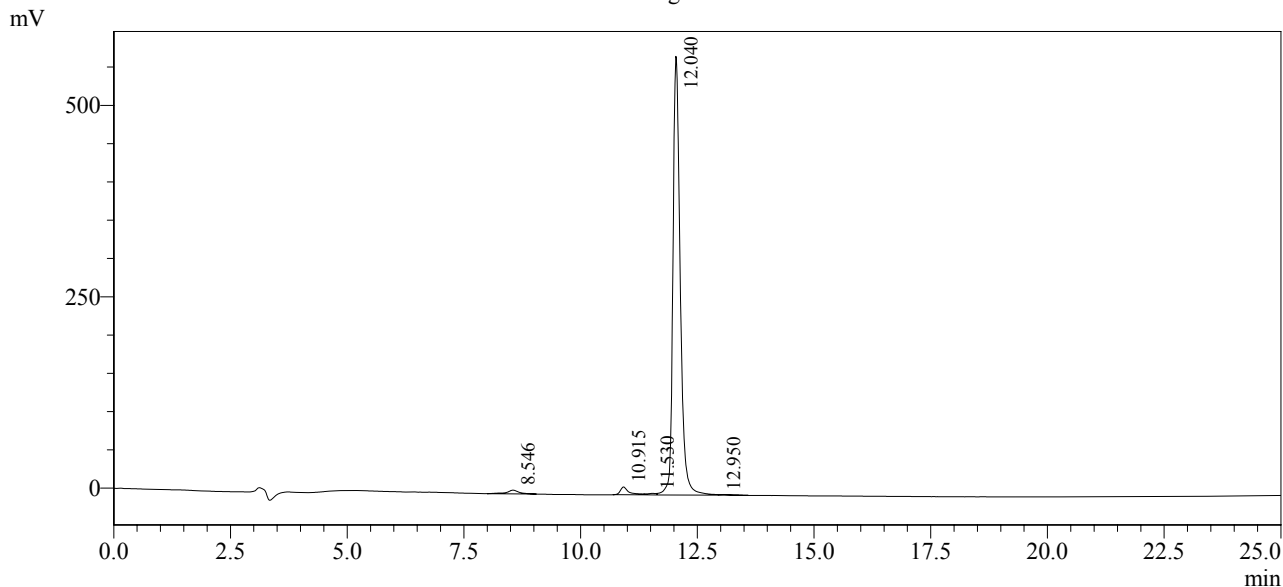

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	8.546	87645	4784	1.348
2	10.915	130353	10156	2.005
3	11.530	28625	1947	0.440
4	12.040	6237443	573136	95.943
5	12.950	17156	847	0.264
Total		6501223	590870	100.000