

Sample Name :[Arg8]-Vasotocin
 Cat No. : RP10061
 Lot No. : E5571519J
 Time Processed : 21:27:05
 Month-Day-Year Processed : 10/16/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow: 1 ml/min
 Wavelength: 220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Pump B Conc.	5
25.00	Pumps	Pump B Conc.	65
25.01	Pumps	Pump B Conc.	95
27.00	Pumps	Pump B Conc.	95
27.01	Pumps	Pump B Conc.	5
32.00	Pumps	Pump B Conc.	5
32.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm
 Equipment: GK12010012

<Chromatogram>

mV

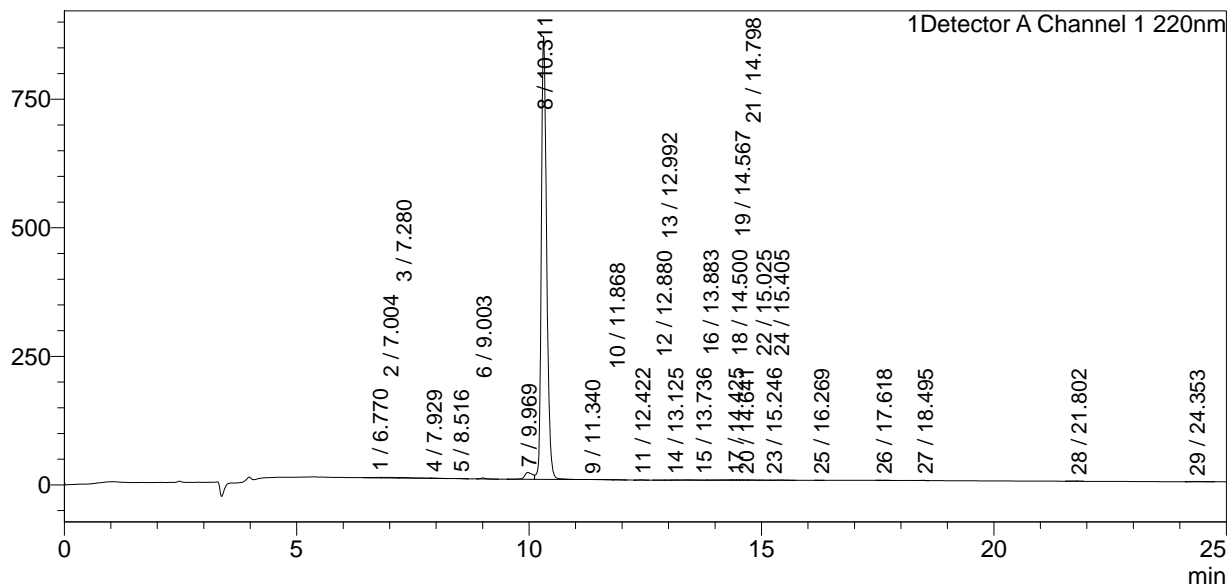

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	6.770	9946	670	0.138
2	7.004	18553	882	0.257
3	7.280	15059	951	0.209
4	7.929	1449	91	0.020
5	8.516	2730	454	0.038
6	9.003	12789	1928	0.177
7	9.969	159886	13350	2.217
8	10.311	6870097	861275	95.255
9	11.340	5917	246	0.082
10	11.868	1299	176	0.018
11	12.422	5571	600	0.077
12	12.880	2824	252	0.039
13	12.992	1721	277	0.024
14	13.125	3070	371	0.043
15	13.736	28517	919	0.395

Peak#	Ret. Time	Area	Height	Area%
16	13.883	20714	866	0.287
17	14.425	2656	491	0.037
18	14.500	2313	522	0.032
19	14.567	2388	541	0.033
20	14.641	3135	534	0.043
21	14.798	7263	554	0.101
22	15.025	5236	438	0.073
23	15.246	2205	386	0.031
24	15.405	8836	686	0.123
25	16.269	1014	123	0.014
26	17.618	1570	168	0.022
27	18.495	2925	476	0.041
28	21.802	5474	633	0.076
29	24.353	7180	522	0.100
Total		7212336	889381	100.000