

Sample Name : [Arg<sup>8</sup>]-Vasotocin

Cat. No. : RP10061 Lot. No. : PE5011804

Pump A : 0.065% trifluoroacetic in 100% water (v/v)

Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)

Total Flow: 1 ml/min

Wavelength: 220 nm


Time	Unit	Command	Value	Comment
0.01	Pumps	Pump A B.Conc	5	
25.00	Pumps	Pump A B.Conc	65	
25.01	Pumps	Pump A B.Conc	95	
31.00	Pumps	Pump A B.Conc	95	
31.01	Pumps	Pump A B.Conc	5	
40.00	Pumps	Pump A B.Conc	5	
40.01	Controller	Stop		

<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

Chromatogram

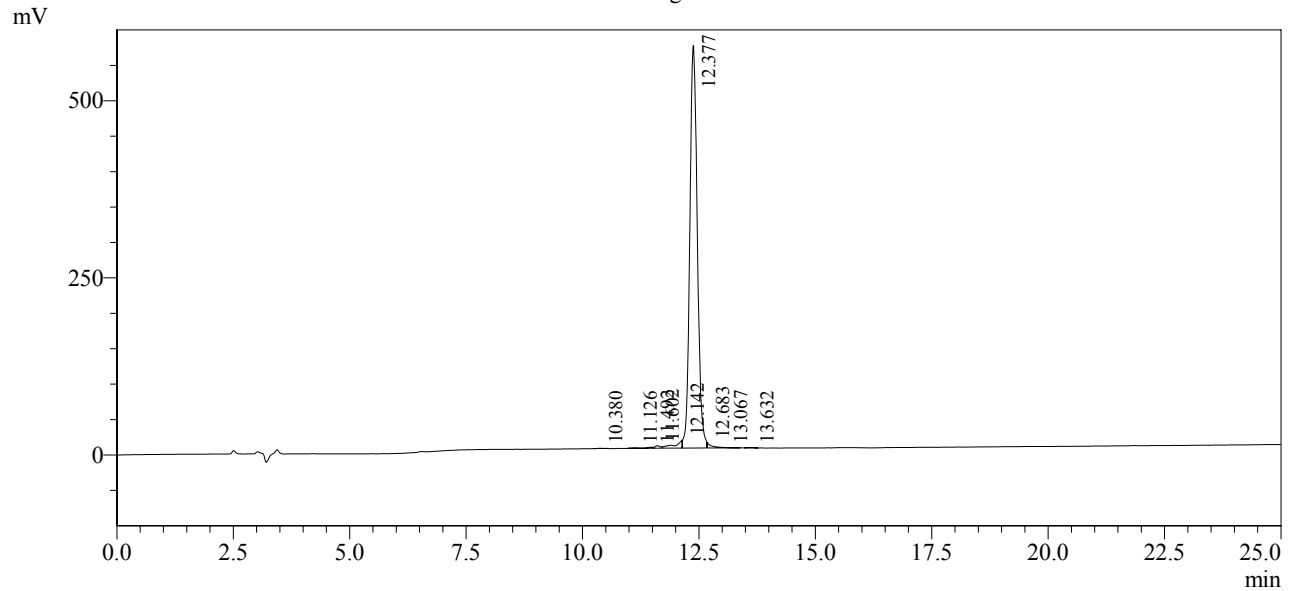

1 Det.A Ch1 / 220nm

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	10.380	2811	361	0.043
2	11.126	6804	537	0.104
3	11.492	11766	1386	0.179
4	11.602	28349	3622	0.432
5	12.142	116982	11385	1.781
6	12.377	6342629	568629	96.588
7	12.683	50297	7156	0.766
8	13.067	4367	582	0.067
9	13.632	2706	402	0.041
Total		6566712	594060	100.000