

Sample Name : [Arg⁸]-Vasotocin
 Cat. No. : RP10061
 Lot. No. : E1703819J
 Time Processed :7:35:44
 Month-Day-Year Processed :10/24/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

Time	Unit	Command	Value	Comment
0.01	Pumps	Pump A B.Conc	5	
25.00	Pumps	Pump A B.Conc	65	
25.01	Pumps	Pump A B.Conc	95	
27.00	Pumps	Pump A B.Conc	95	
27.01	Pumps	Pump A B.Conc	5	
35.00	Pumps	Pump A B.Conc	5	
35.01	Controller	Stop		


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

Equipment: GK11010009

Chromatogram

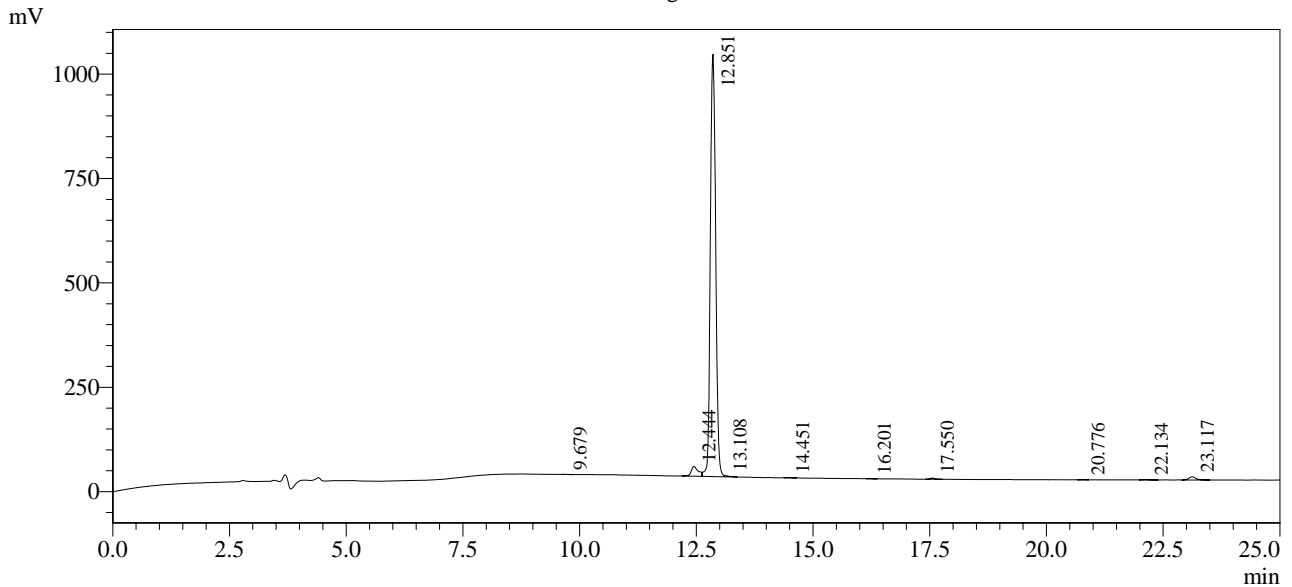

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	9.679	1594	277	0.019
2	12.444	251795	23419	2.991
3	12.851	8035692	1011495	95.452
4	13.108	17436	2780	0.207
5	14.451	3238	451	0.038
6	16.201	2287	405	0.027
7	17.550	18503	2626	0.220
8	20.776	2192	312	0.026
9	22.134	6294	503	0.075
10	23.117	79550	7491	0.945
Total		8418581	1049761	100.000