

Sample Name : Urocortin III, mouse
 Cat. No. : RP10101
 Lot. No. : E5581419J
 Time Processed : 23:47:50
 Month-Day-Year Processed : 10/21/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow: 1 ml/min
 Wavelength: 220 nm

Time	Unit	Command	Value	Comment
0.01	Pumps	Pump A B.Conc	15	
25.00	Pumps	Pump A B.Conc	75	
25.01	Pumps	Pump A B.Conc	95	
31.00	Pumps	Pump A B.Conc	95	
31.01	Pumps	Pump A B.Conc	15	
40.00	Pumps	Pump A B.Conc	15	
40.01	Controller	Stop		


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

Equipment: GK11010009

Chromatogram

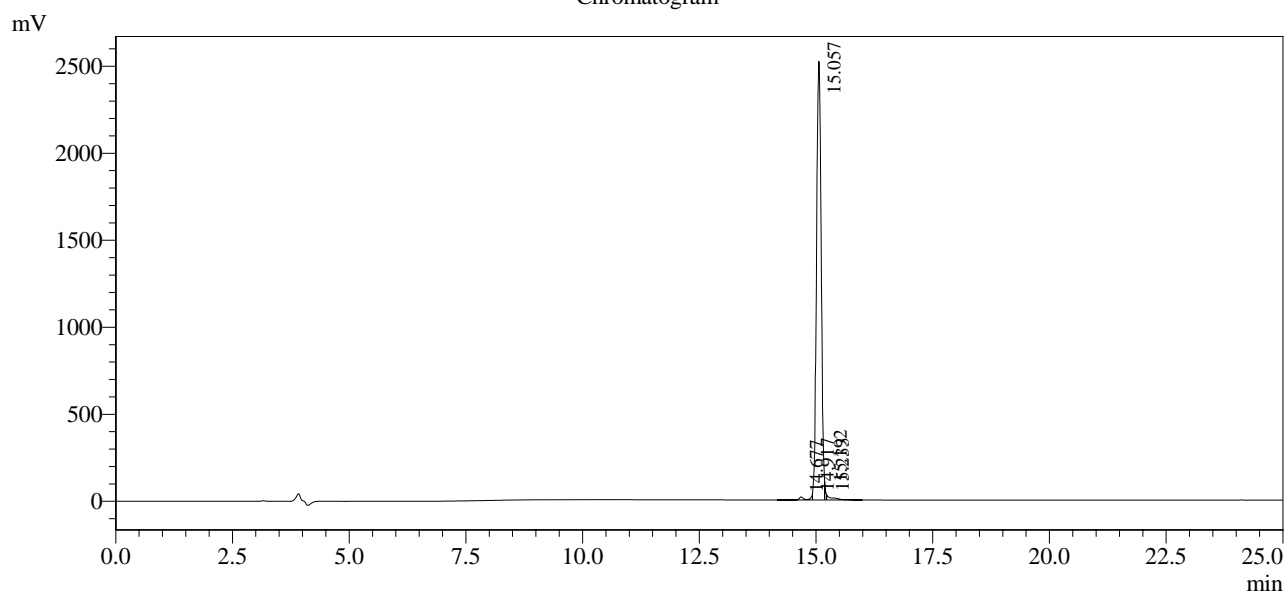

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	14.677	116336	17516	0.642
2	14.917	67120	26215	0.370
3	15.057	17584792	2521270	97.018
4	15.192	121684	75863	0.671
5	15.233	235310	25925	1.298
Total		18125242	2666789	100.000