

Sample Name :Urocortin II, human
 Cat No.: RP10098
 Lot No.:E3642220A
 Time Processed :8:44:01
 Month-Day-Year Processed :02/06/2020

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Pump A B.Conc	15
25.00	Pumps	Pump A B.Conc	75
25.01	Pumps	Pump A B.Conc	95
31.00	Pumps	Pump A B.Conc	95
31.01	Pumps	Pump A B.Conc	15
40.00	Pumps	Pump A B.Conc	15
40.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm
 Equipment:ZJ19010324

<Chromatogram>

mV

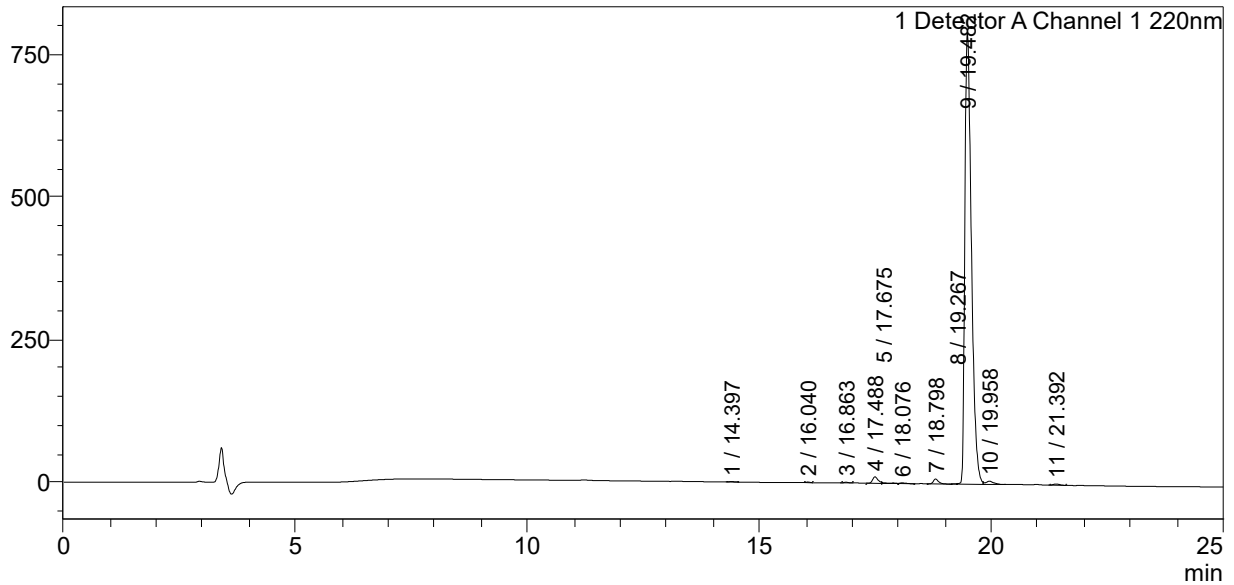

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	14.397	5097	884	0.063
2	16.040	5708	1037	0.070
3	16.863	8141	1307	0.100
4	17.488	95591	11408	1.175
5	17.675	15369	1154	0.189
6	18.076	12351	1429	0.152
7	18.798	71296	8902	0.876
8	19.267	6876	1030	0.085
9	19.482	7830171	792292	96.231
10	19.958	65258	5786	0.802
11	21.392	20987	2146	0.258
Total		8136846	827374	100.000