

Sample Name :  $\beta$ -Amyloid (1-42), human  
 Cat. No. : RP10017  
 Lot. No. : PE3561612

Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
 Total Flow: 1 ml/min  
 Wavelength: 220 nm


Time	Unit	Command	Value	Comment
0.01	Pumps	Pump B Conc.	10	
25.00	Pumps	Pump B Conc.	100	
25.01	Pumps	Pump B Conc.	95	
32.00	Pumps	Pump B Conc.	95	
32.01	Pumps	Pump B Conc.	5	
40.00	Pumps	Pump B Conc.	5	
40.01	Controller	Stop		

<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

Chromatogram

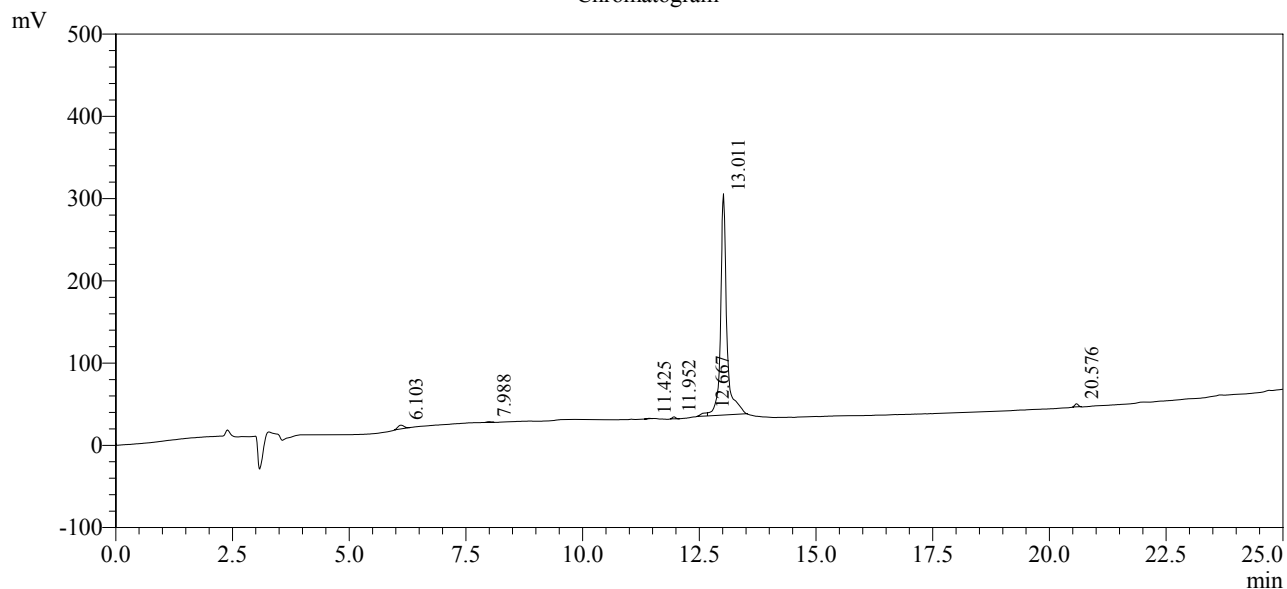

1 Det. A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	6.103	42350	4610	1.639
2	7.988	3877	656	0.150
3	11.425	2554	568	0.099
4	11.952	11686	2399	0.452
5	12.667	36233	3747	1.403
6	13.011	2466997	269088	95.505
7	20.576	19403	3704	0.751
Total		2583101	284772	100.000