


Mass Spectrum

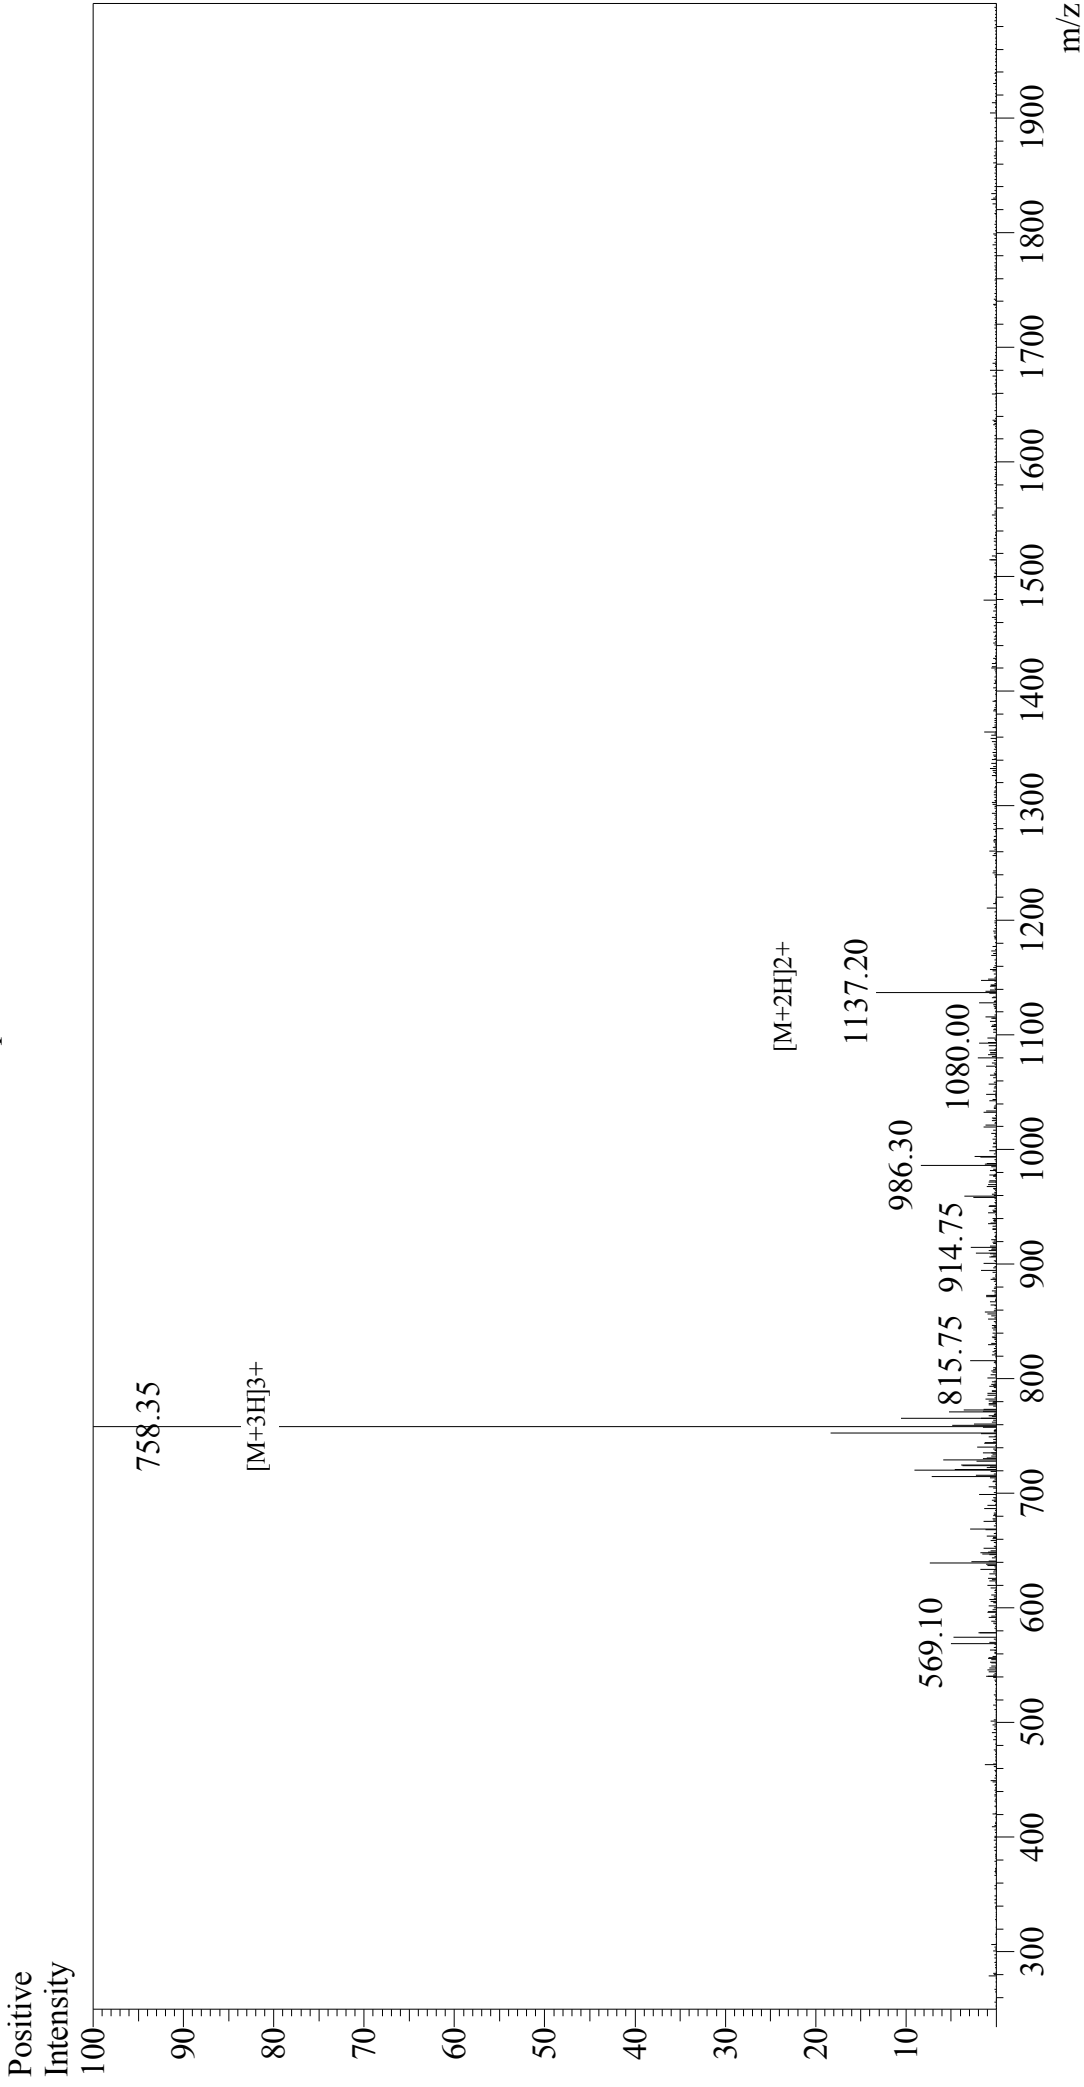

Sample Information

Acquired by : Gary
 Month-Day Processed : 09/20/17
 Time Processed : 12:12:15
 Injection Volume : 0.2
 Sample Name : Flagelin22
 Cat No. : RP19986
 Lot No. : PE2441709
 Theoretical MW : 2272.50
 Observed MW : 2272.05

Interface : ESI
 Nebulizing Gas Flow : 1.5L/min
 CDL Temp : 250°C
 Block Temp : 200°C

Interface Bias : +4.5 kV
 Drying Gas Flow : 5 L/min
 T.Flow : 0.2 ml/min
 B.conc : 50% H₂O/50% MeOH