

Sample Name : Urocortin II, human

Cat No.: RP10098

Lot No. : PE7031901

Time Processed : 8:52:45

Month-Day-Year Processed : 04/24/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)

Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)

Total Flow: 1 ml/min

Wavelength: 220 nm

Time	Unit	Command	Value	Comment
0.01	Pumps	Pump B Conc.	20	
25.00	Pumps	Pump B Conc.	80	
25.01	Pumps	Pump B Conc.	95	
30.00	Pumps	Pump B Conc.	95	
30.01	Pumps	Pump B Conc.	20	
35.00	Pumps	Pump B Conc.	20	
35.01	Controller	Stop		


<<Column Performance>>

<Detector A>

Column : Alltima™ C18 4.6 x 250 mm

Equipment: GR09010180

Chromatogram

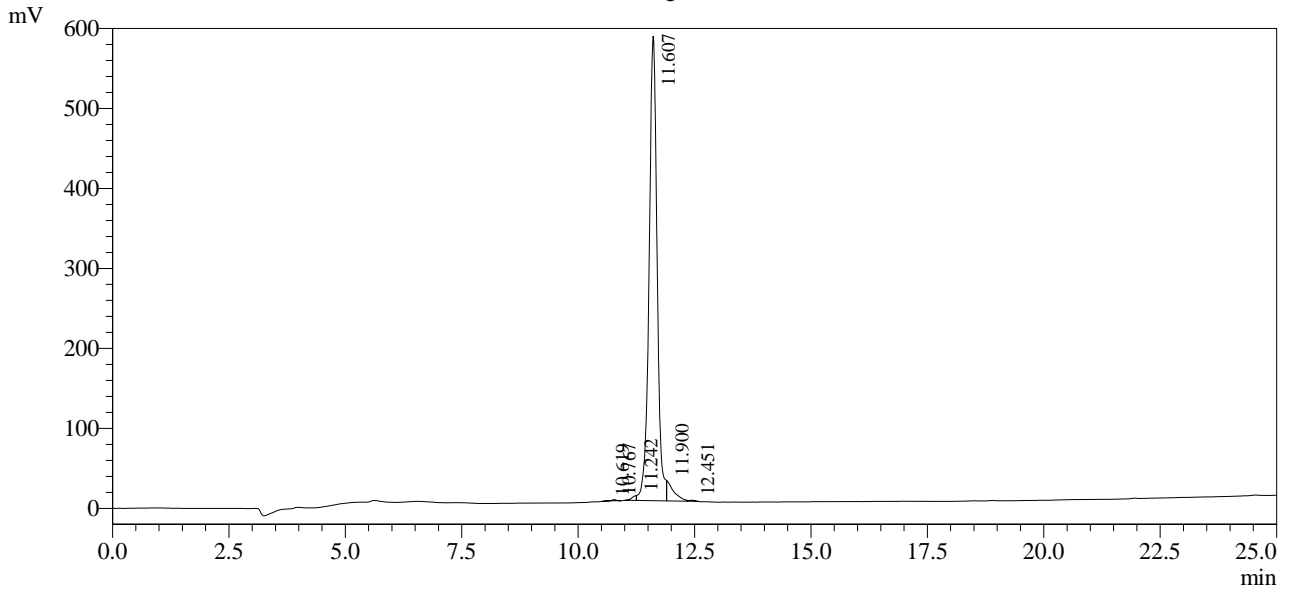

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	10.619	1831	252	0.025
2	10.767	8630	1459	0.119
3	11.242	39049	6011	0.537
4	11.607	6955685	580698	95.588
5	11.900	258610	25465	3.554
6	12.451	12902	1366	0.177
Total		7276707	615250	100.000