

Sample Name:Flagelin22
 Cat No. :RP19986
 Lot No.:E6040020C
 Time Processed: 5:14:06 AM
 Month-Day-Year Processed :03/28/2020

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Pump A B.Conc	5
25.00	Pumps	Pump A B.Conc	65
25.01	Pumps	Pump A B.Conc	95
31.00	Pumps	Pump A B.Conc	95
31.01	Pumps	Pump A B.Conc	5
40.00	Pumps	Pump A B.Conc	5
40.00	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Alltima™ C18 4.6 x 250 mm
 Equipment:ZJ19010325

<Chromatogram>

mV

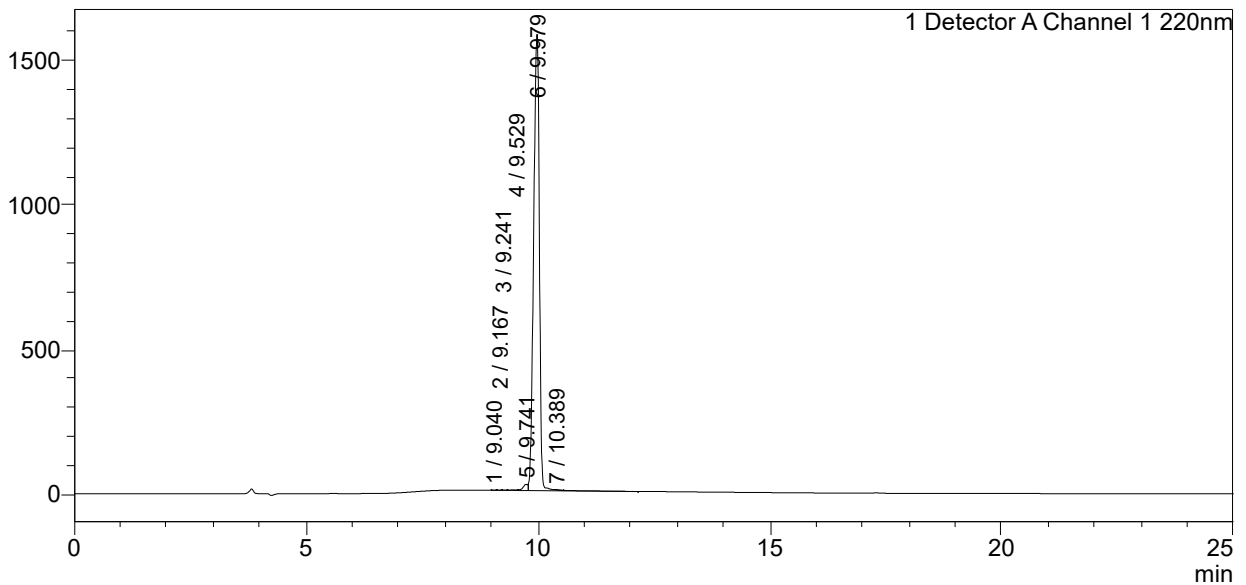

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	9.040	464	98	0.003
2	9.167	1261	228	0.009
3	9.241	3241	344	0.024
4	9.529	21241	2159	0.156
5	9.741	136960	21163	1.003
6	9.979	13487182	1581065	98.785
7	10.389	2655	570	0.019
Total		13653003	1605628	100.000