

Sample Name : Flagelin22
 Cat. No. : RP19986
 Lot. No. : PE3131611

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm


Time	Unit	Command	Value	Comment
0.01	Pumps	Pump A B.Conc	5	
25.00	Pumps	Pump A B.Conc	65	
25.01	Pumps	Pump A B.Conc	95	
31.00	Pumps	Pump A B.Conc	95	
31.01	Pumps	Pump A B.Conc	5	
40.00	Pumps	Pump A B.Conc	5	
40.01	Controller	Stop		

<<Column Performance>>

<Detector A>

Column : Alltima™ C18 4.6 x 250 mm

Chromatogram

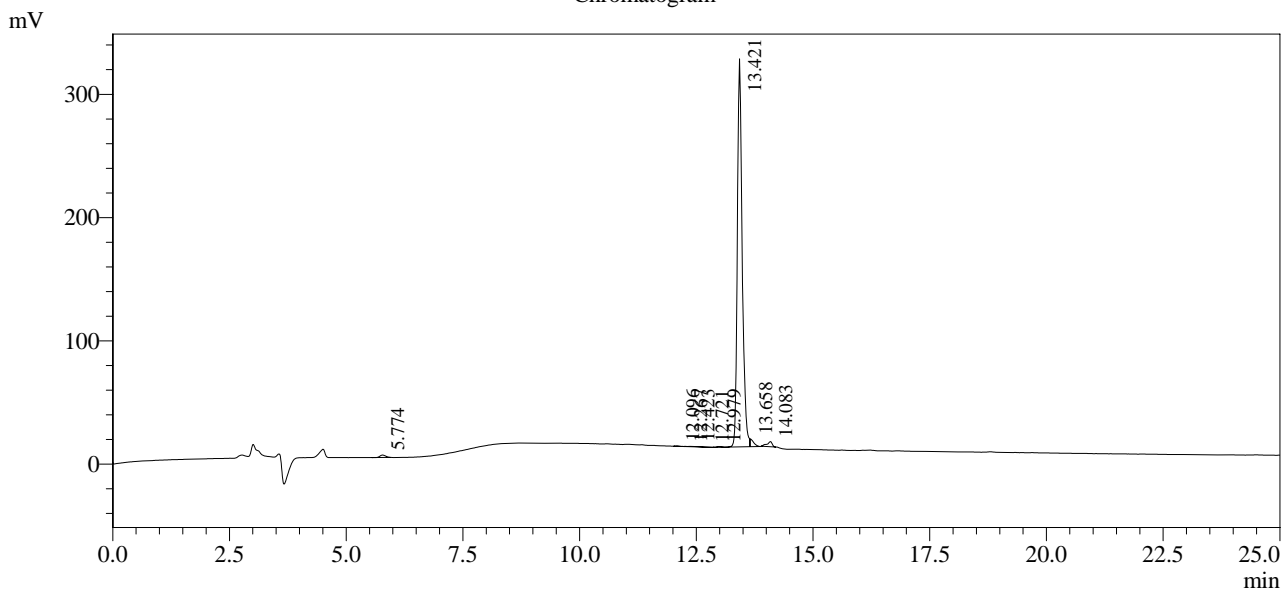

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	5.774	15624	1935	0.658
2	12.096	1049	162	0.044
3	12.267	746	108	0.031
4	12.423	3335	426	0.140
5	12.721	816	154	0.034
6	12.979	4250	643	0.179
7	13.421	2284707	314755	96.209
8	13.658	31604	6163	1.331
9	14.083	32592	4156	1.372
Total		2374723	328504	100.000