

Sample Name : Flagelin 22
 Cat No.:RP19986
 Lot No.:E6829620H
 Time Processed :12:46:46
 Month-Day-Year Processed :08/15/2020

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm


<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Solvent B Conc.	5
25.00	Pumps	Solvent B Conc.	65
25.01	Pumps	Solvent B Conc.	95
31.00	Pumps	Solvent B Conc.	95
31.01	Pumps	Solvent B Conc.	5
40.00	Pumps	Solvent B Conc.	5
40.01	Controller	Stop	

<<Column Performance>>

<Detector A>
 Column : Inertsil ODS-3 4.6 x 250 mm
 Equipment:ZJ19010324

<Chromatogram>

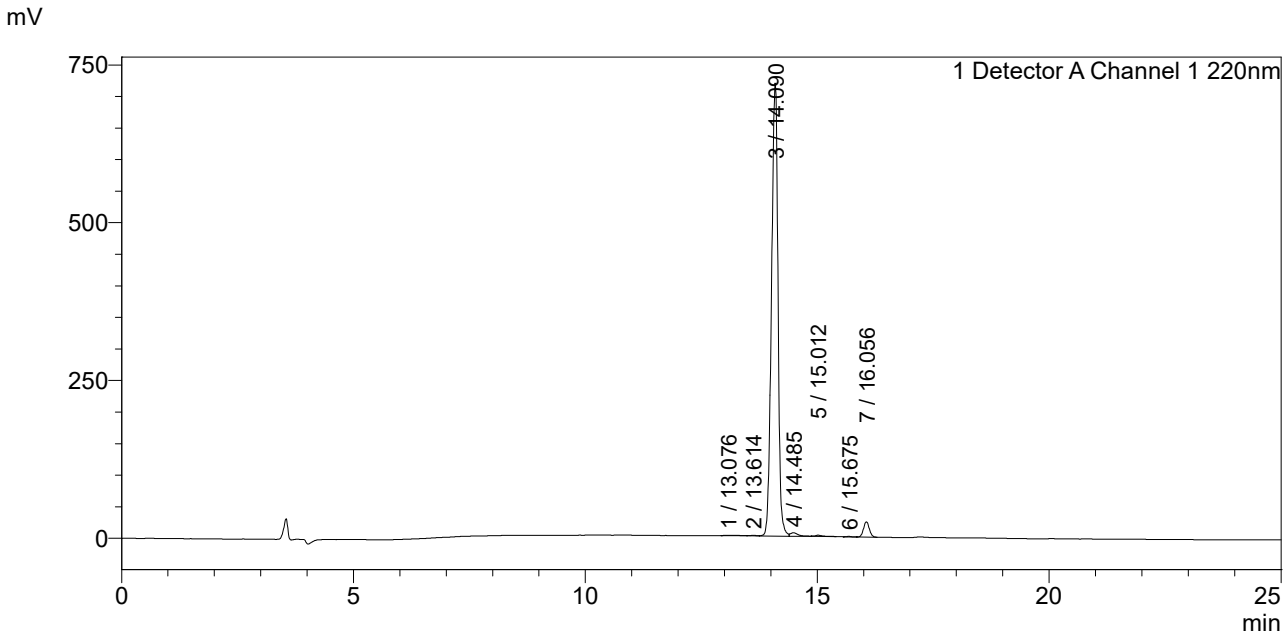

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	13.076	13272	619	0.183
2	13.614	8013	698	0.110
3	14.090	6921078	718013	95.417
4	14.485	67188	5592	0.926
5	15.012	27877	2212	0.384
6	15.675	5138	838	0.071
7	16.056	210934	24304	2.908
Total		7253499	752276	100.000