

Sample Name : β -Amyloid (42-1)
 Cat No. : RP10034
 Lot No. : PE6881809
 Time Processed : 13:46:37
 Month-Day-Year Processed : 09/26/2018
 Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow: 1 ml/min
 Wavelength: 220 nm

Time	Unit	Command	Value	Comment
0.01	Pumps	Pump B Conc.	20	
25.00	Pumps	Pump B Conc.	80	
25.01	Pumps	Pump B Conc.	95	
30.00	Pumps	Pump B Conc.	95	
30.01	Pumps	Pump B Conc.	20	
35.00	Pumps	Pump B Conc.	20	
35.01	Controller	Stop		


<<Column Performance>>

<Detector A>

Column : AlltimaTM C18 4.6 x 250 mm

Equipment: GR09010180

Chromatogram

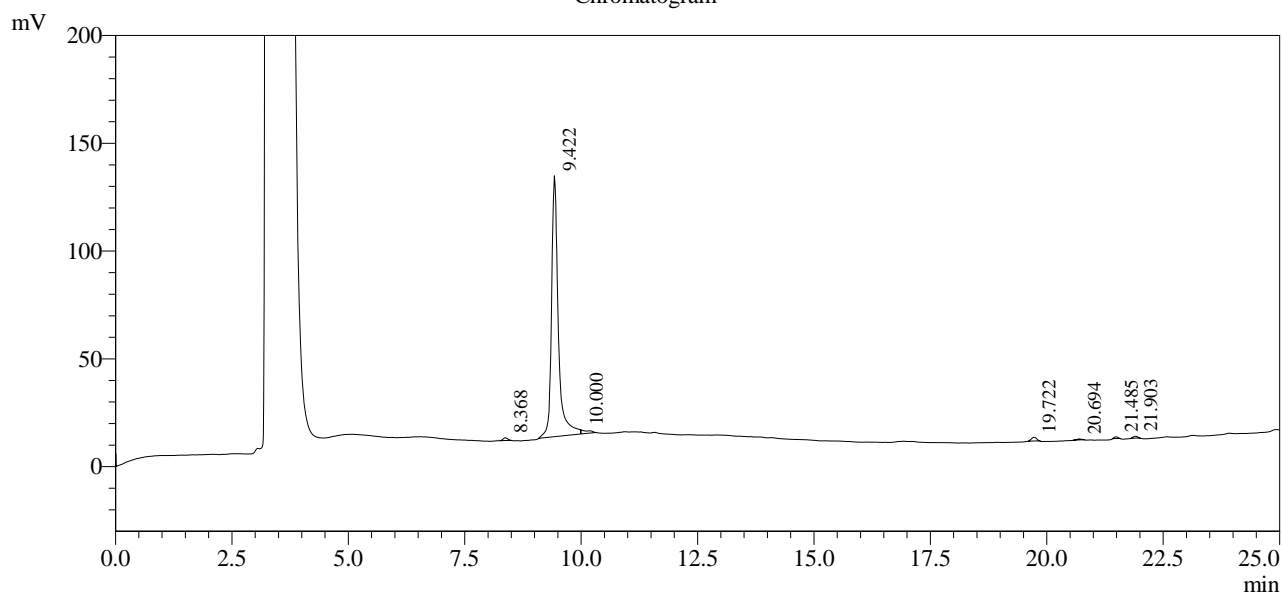

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	8.368	8350	1220	0.653
2	9.422	1224722	121034	95.815
3	10.000	18687	1817	1.462
4	19.722	12887	1721	1.008
5	20.694	3316	458	0.259
6	21.485	4462	800	0.349
7	21.903	5796	903	0.453
Total		1278219	127953	100.000