

Sample Name : $\beta$ -Amyloid (42-1)  
 Cat No :RP10034  
 Lot No :E4689519I  
 Time Processed :5:31:56 PM  
 Month-Day-Year Processed :12/03/2020

Pump A : 0.5% Ammonia solution in 100% water (v/v)  
 Pump B : 0.2% Ammonia solution in 100% acetonitrile (v/v)  
 Total Flow:1 ml/min  
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Pump A B.Conc	5
25.00	Pumps	Pump A B.Conc	65
25.01	Pumps	Pump A B.Conc	95
27.00	Pumps	Pump A B.Conc	95
27.01	Pumps	Pump A B.Conc	5
35.00	Pumps	Pump A B.Conc	5
35.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column :UniPS 10-300 4.6 x 250 mm  
 Equipment: SS-CM-0309

### <Chromatogram>

mV

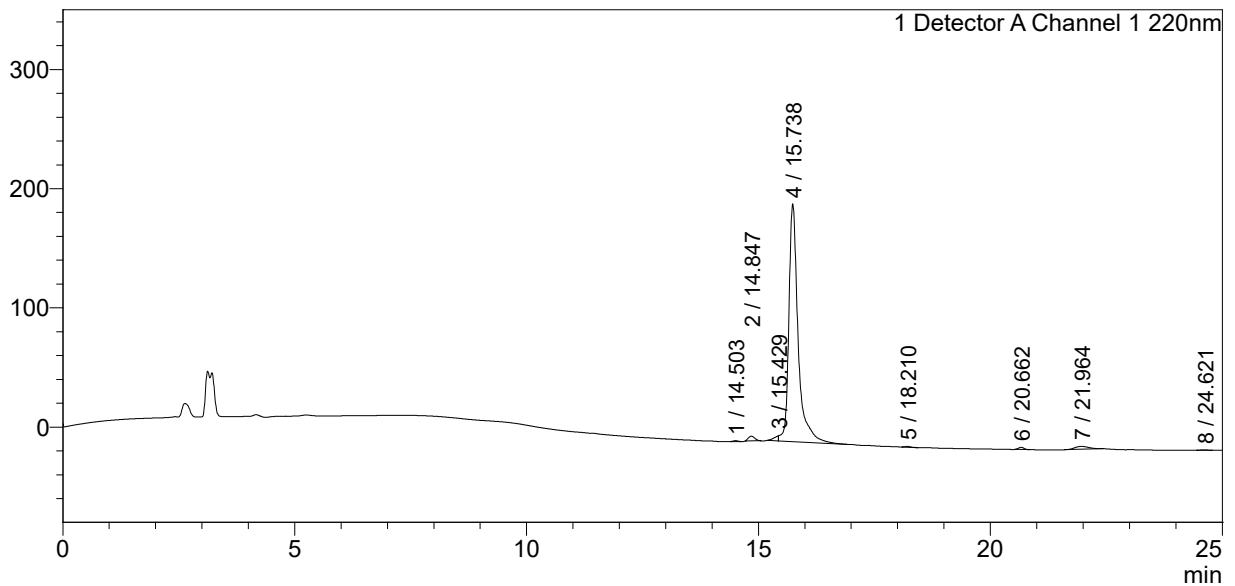

### <Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	14.503	5033	689	0.173
2	14.847	36710	3838	1.261
3	15.429	28434	4118	0.977
4	15.738	2766086	199439	95.050
5	18.210	5036	647	0.173
6	20.662	14145	1756	0.486
7	21.964	52103	2478	1.790
8	24.621	2592	225	0.089
Total		2910138	213190	100.000