

Sample Name:β-Amyloid (42-1)
 Cat No. :RP10034
 Lot No. :E8353421F
 Time Processed :4:10:35 PM
 Month-Day-Year Processed :08/13/2021

Pump A : 0.1% Ammonia solution in 100% water (v/v)
 Pump B :0.1% Ammonia solution in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Pump A B.Conc	5
25.00	Pumps	Pump A B.Conc	65
25.01	Pumps	Pump A B.Conc	95
27.00	Pumps	Pump A B.Conc	95
27.01	Pumps	Pump A B.Conc	5
35.00	Pumps	Pump A B.Conc	5
35.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column :Inertsil ODS-3 4.6 x 250 mm
 Equipment: ZJ19010141

<Chromatogram>

mV

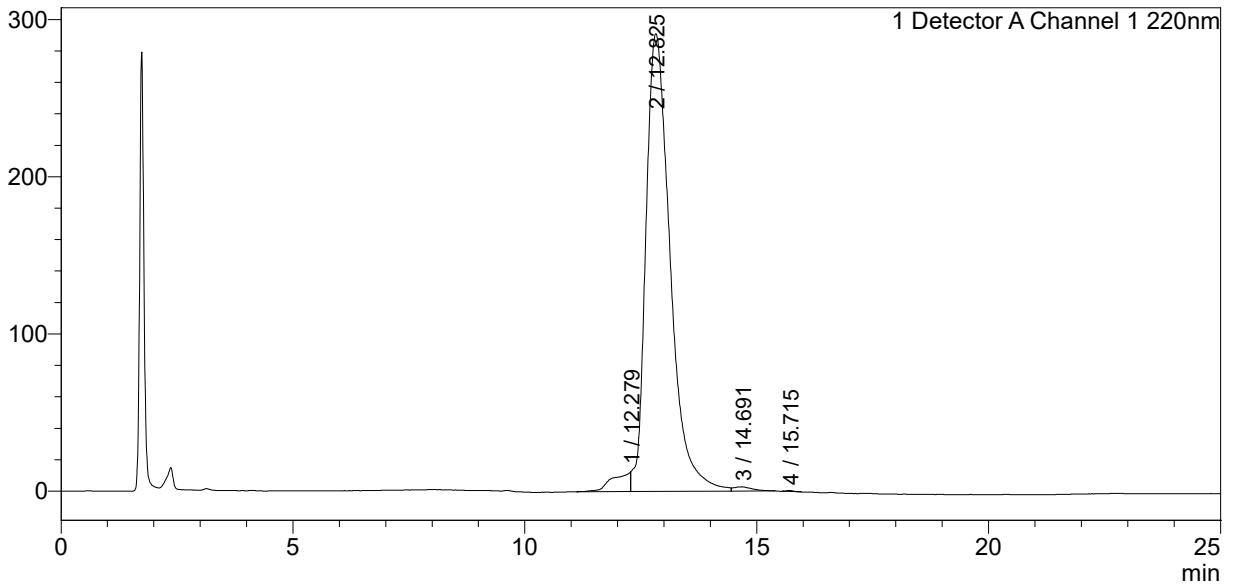

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	12.279	336829	12300	3.066
2	12.825	10570807	291243	96.207
3	14.691	73411	2662	0.668
4	15.715	6534	653	0.059
Total		10987582	306857	100.000