

Sample Name :Urocortin II, human  
Cat No.: RP10098  
Lot No.:E5492920A  
Time Processed :10:49:17  
Month-Day-Year Processed :02/03/2020

Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
Total Flow:1 ml/min  
Wavelength:220 nm

<<LC Time Program>>


Time	Module	Command	Value
0.01	Pumps	Pump A B.Conc	15
25.00	Pumps	Pump A B.Conc	75
25.01	Pumps	Pump A B.Conc	95
31.00	Pumps	Pump A B.Conc	95
31.01	Pumps	Pump A B.Conc	15
40.00	Pumps	Pump A B.Conc	15
40.01	Controller	Stop	

<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm  
Equipment:ZJ19010324

### <Chromatogram>

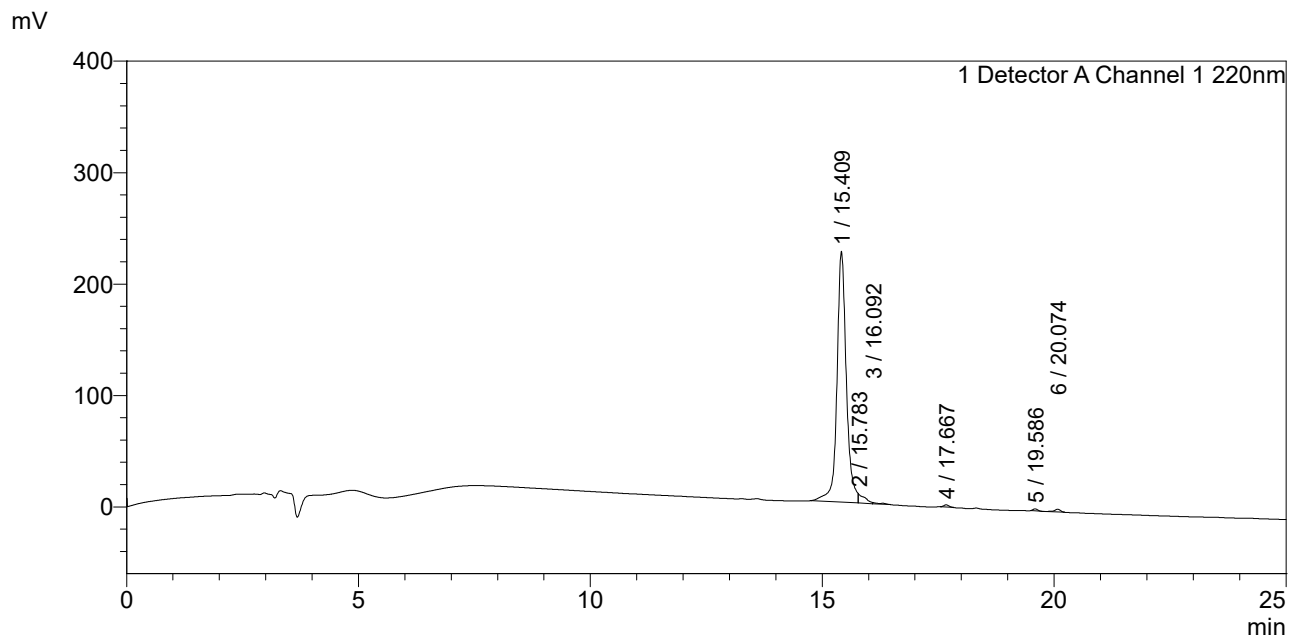

### <Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	15.409	3160165	225201	95.714
2	15.783	79419	8118	2.405
3	16.092	12392	1056	0.375
4	17.667	14907	1956	0.452
5	19.586	11648	1743	0.353
6	20.074	23152	2461	0.701
Total		3301683	240535	100.000