

Sample Name : β -Amyloid (42-1)
 Cat. No. : RP10034
 Lot. No. : E3613319K
 Time Processed : 17:56:53
 Month-Day-Year Processed : 01/16/2020

Pump A : 0.5% Ammonia solution in 100% water (v/v)
 Pump B : 0.2% Ammonia solution in 100% acetonitrile (v/v)
 Total Flow: 1 ml/min
 Wavelength: 220 nm


Time	Unit	Command	Value	Comment
0.01	Pumps	Pump B Conc.	5	
25.00	Pumps	Pump B Conc.	65	
25.01	Pumps	Pump B Conc.	95	
27.00	Pumps	Pump B Conc.	95	
27.01	Pumps	Pump B Conc.	5	
35.00	Pumps	Pump B Conc.	5	
35.01	Controller	Stop		

<<Column Performance>>

<Detector A>

Column : UniPS 10-300 4.6 x 250 mm
 Equipment : SS-CM-0310

Chromatogram

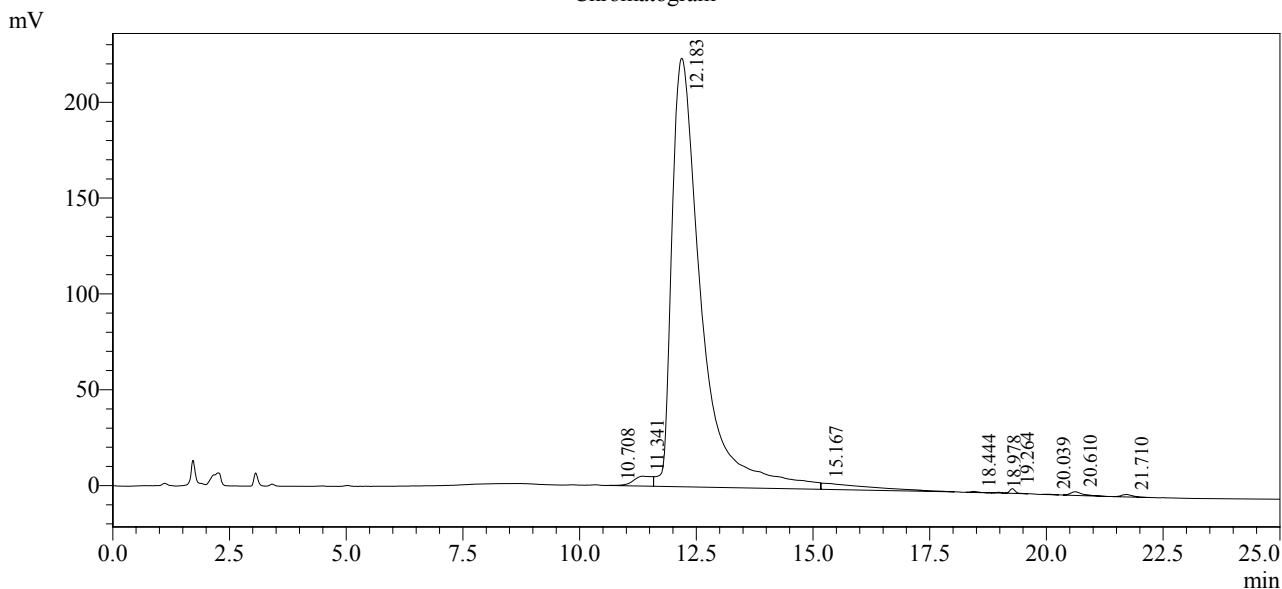

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	10.708	1652	161	0.016
2	11.341	143426	5163	1.395
3	12.183	9818033	223613	95.486
4	15.167	231258	3368	2.249
5	18.444	6385	556	0.062
6	18.978	3207	411	0.031
7	19.264	20187	2449	0.196
8	20.039	1856	169	0.018
9	20.610	35061	1901	0.341
10	21.710	21089	1302	0.205
Total		10282154	239094	100.000