

Sample Name : β -Amyloid (1-42), human
 Cat. No. : RP10017
 Lot. No. : PE5881904
 Time Processed : 11:30:44
 Month-Day-Year Processed : 07/05/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow: 1 ml/min
 Wavelength: 220 nm

Time	Unit	Command	Value	Comment
0.01	Pumps	Pump A B.Conc	10	
25.00	Pumps	Pump A B.Conc	100	
25.01	Pumps	Pump A B.Conc	95	
31.00	Pumps	Pump A B.Conc	95	
31.01	Pumps	Pump A B.Conc	10	
40.00	Pumps	Pump A B.Conc	10	
40.01	Controller	Stop		


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

Equipment: GK11010009

Chromatogram

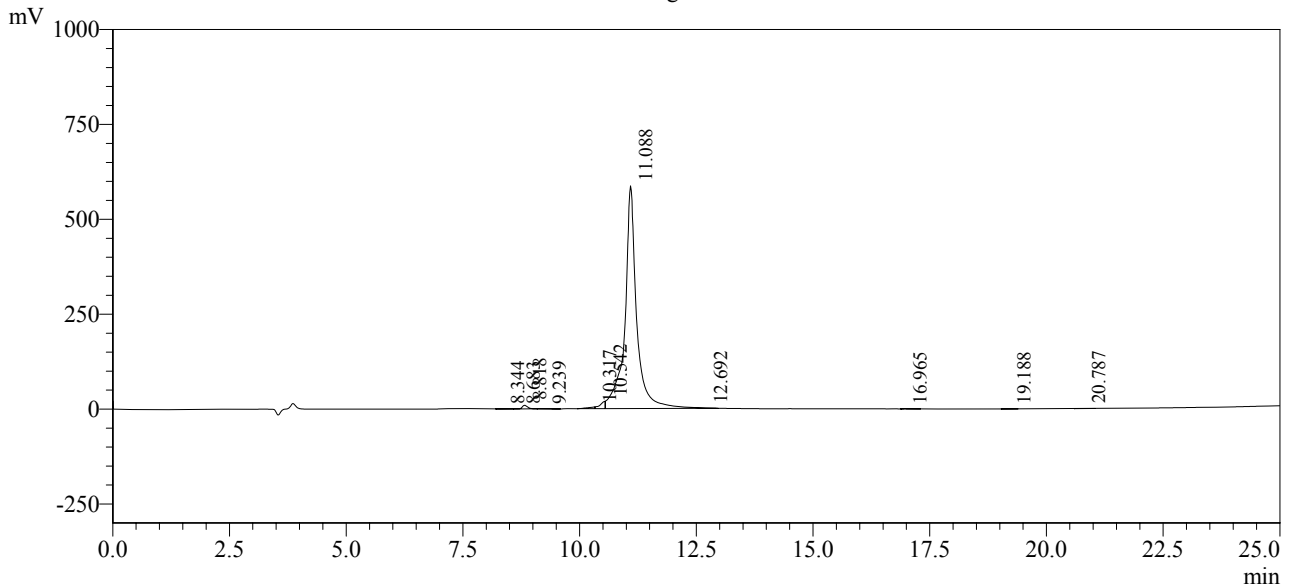

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	8.344	4944	511	0.047
2	8.683	1254	251	0.012
3	8.818	75938	9617	0.716
4	9.239	2984	343	0.028
5	10.317	45970	4433	0.433
6	10.542	147677	19290	1.392
7	11.088	10306849	586627	97.127
8	12.692	8085	859	0.076
9	16.965	4398	525	0.041
10	19.188	2068	290	0.019
11	20.787	11549	1387	0.109
Total		10611715	624133	100.000