


Mass Spectrum

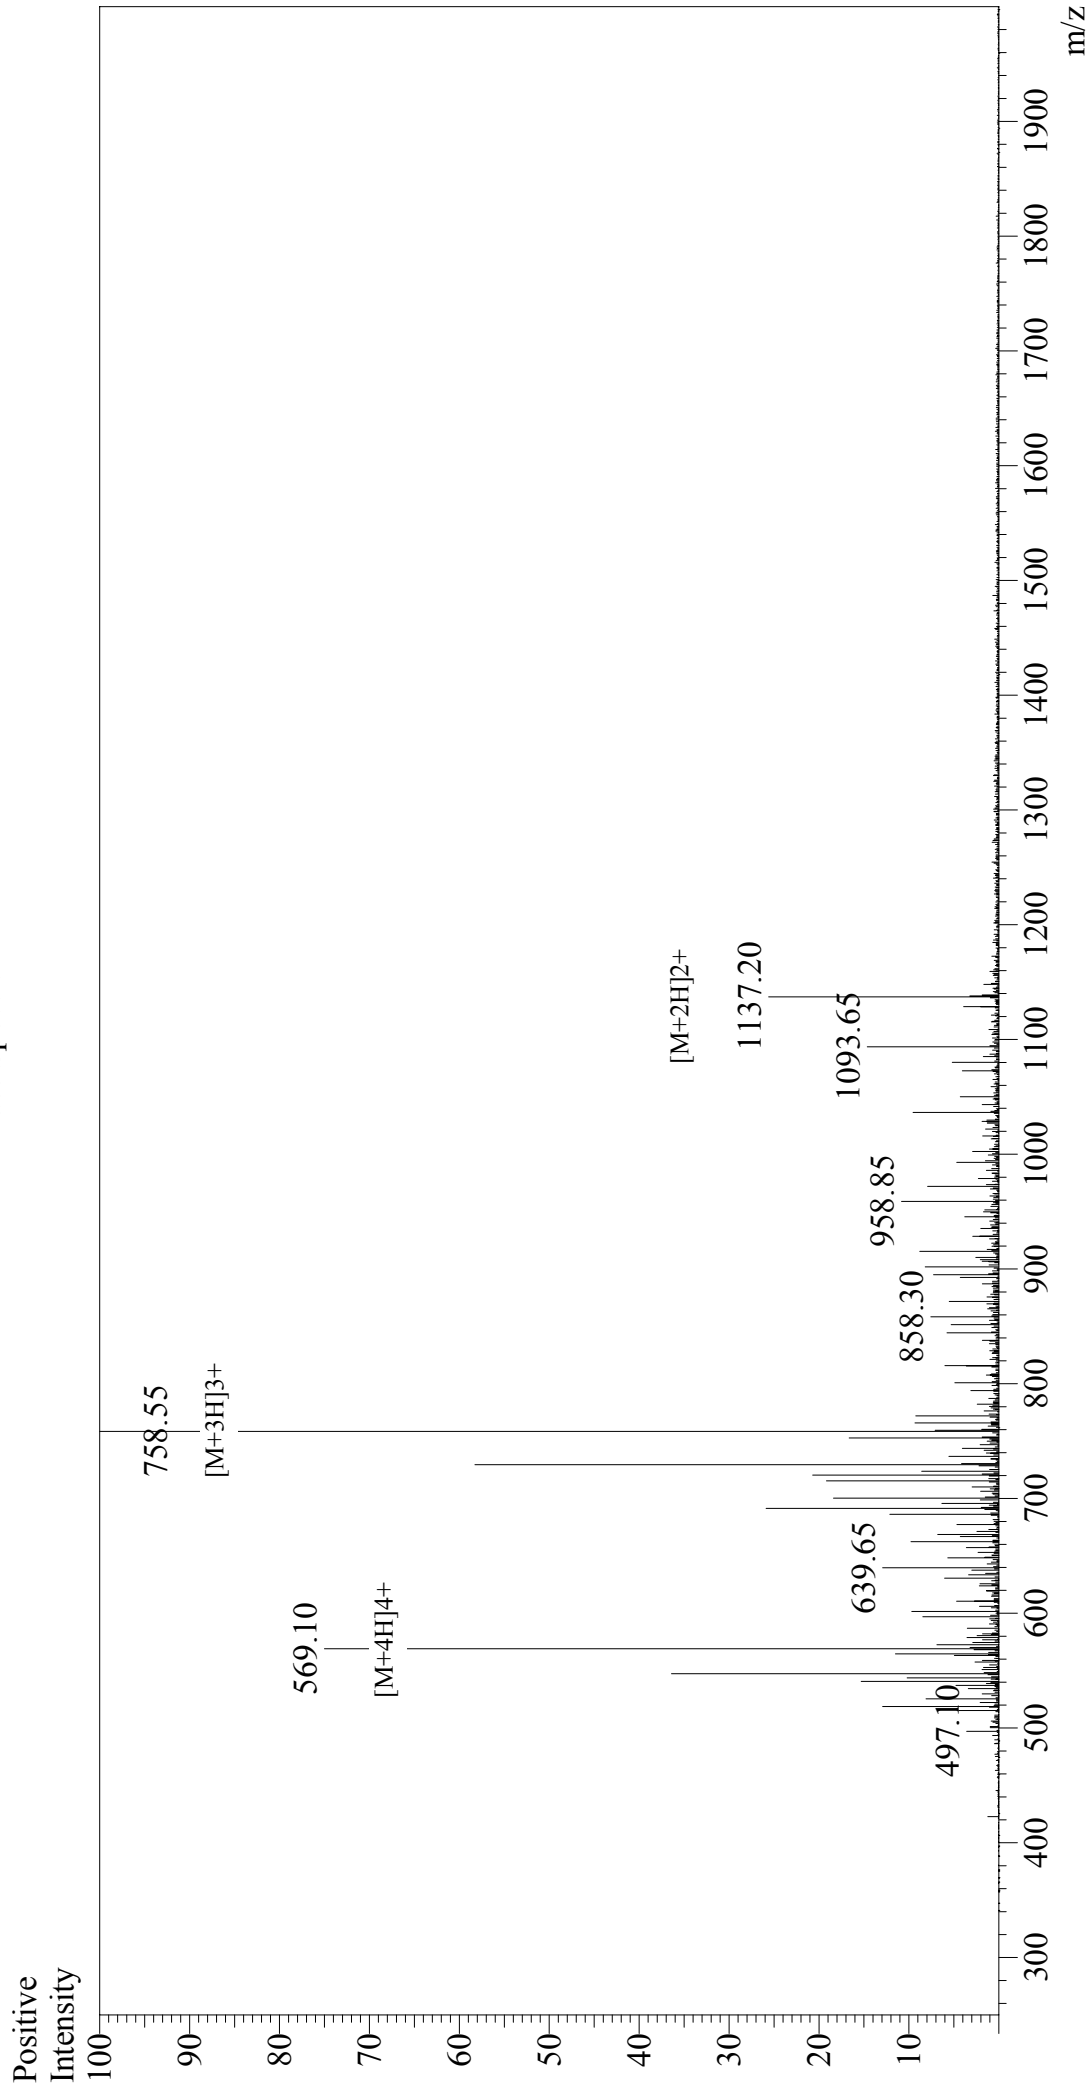

Sample Information

Acquired by : Gary
Month-Day Processed : 12/15/17
Time Processed : 16:57:23
Injection Volume : 0.2
Sample Name : Flagelin22
Cat. No. : RP19986
Lot. No. : PE6591712
Theoretical MW : 2272.50
Observed MW : 2272.65

Interface : ESI
Nebulizing Gas Flow : 1.5L/min
CDL Temp : 250°C
Block Temp : 200°C

Interface Bias : +4.5 kV
Drying Gas Flow : 5 L/min
T.Flow : 0.2 ml/min
B.conc : 50%H2O/50%MeOH