

Sample Name :MOG(35-55)
 Cat. No. : RP10245
 Lot. No. : E4784620B
 Time Processed :10:14:03
 Month-Day-Year Processed :03/04/2020

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

Time	Unit	Command	Value	Comment
0.01	Pumps	Pump A B.Conc	5	
25.00	Pumps	Pump A B.Conc	65	
25.01	Pumps	Pump A B.Conc	95	
27.00	Pumps	Pump A B.Conc	95	
27.01	Pumps	Pump A B.Conc	5	
35.00	Pumps	Pump A B.Conc	5	
35.01	Controller	Stop		


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

Equipment: GR11010440

Chromatogram

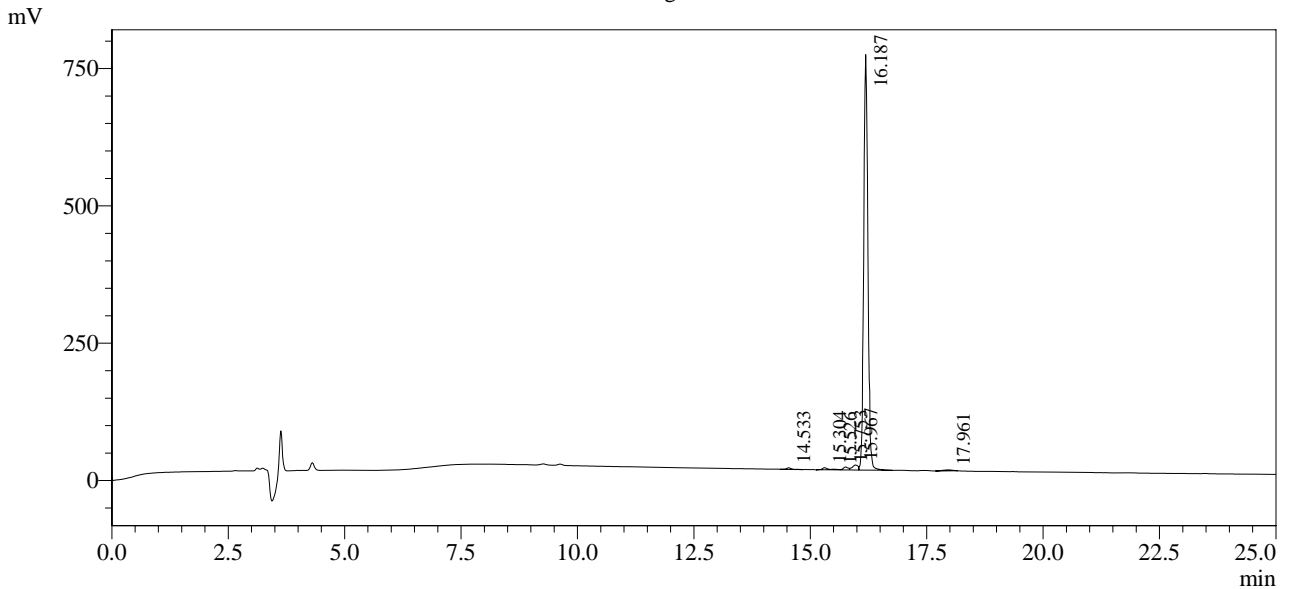

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	14.533	18344	2838	0.371
2	15.304	29065	3841	0.588
3	15.526	10809	1329	0.219
4	15.753	39701	5269	0.803
5	15.967	79230	9209	1.603
6	16.187	4740195	756299	95.915
7	17.961	24727	1725	0.500
Total		4942071	780510	100.000