

Sample Name : MOG(35-55)
 Sample ID : U9776CH270-1

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow: 1 ml/min
 Wavelength: 220 nm


Time	Unit	Command	Value	Comment
0.01	Pumps	Pump A B.Conc	5	
25.00	Pumps	Pump A B.Conc	65	
25.01	Pumps	Pump A B.Conc	95	
31.00	Pumps	Pump A B.Conc	95	
31.01	Pumps	Pump A B.Conc	5	
40.00	Pumps	Pump A B.Conc	5	
40.01	Controller	Stop		

<<Column Performance>>

<Detector A>

Column : AlltimaTM C18 4.6 x 250 mm

Chromatogram

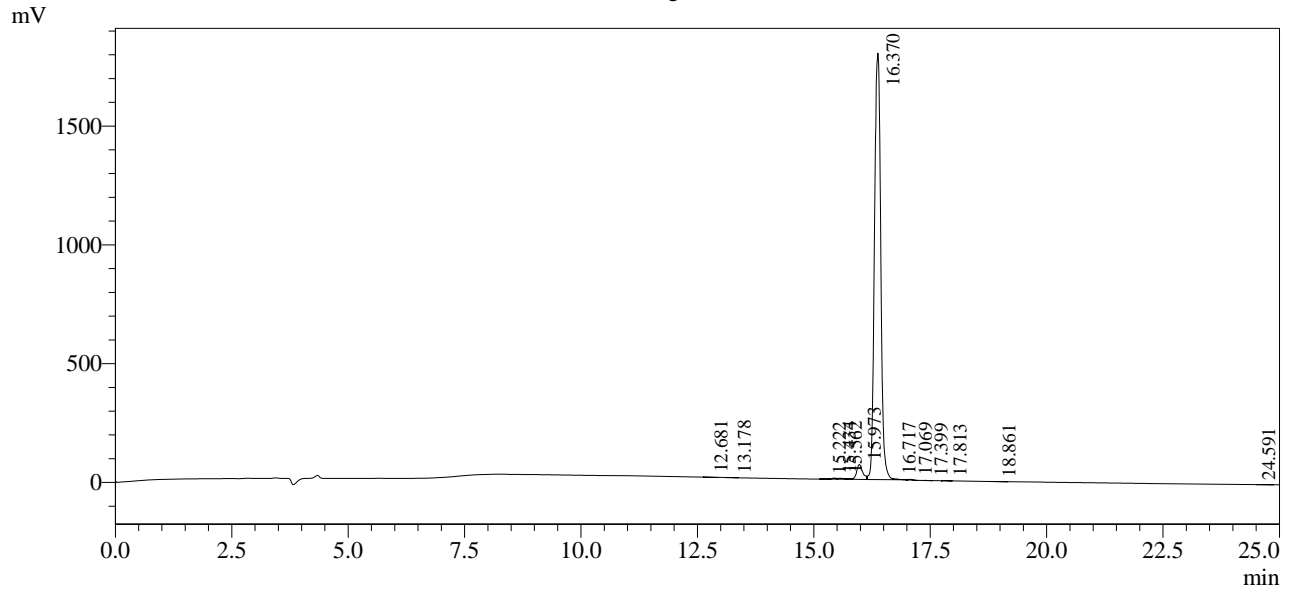

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	12.681	2916	350	0.017
2	13.178	2628	371	0.015
3	15.222	5369	991	0.031
4	15.434	28492	4545	0.162
5	15.562	39494	4104	0.225
6	15.973	572108	62678	3.261
7	16.370	16833452	1794419	95.938
8	16.717	29492	4028	0.168
9	17.069	15330	2780	0.087
10	17.399	2809	456	0.016
11	17.813	4826	825	0.028
12	18.861	5743	364	0.033
13	24.591	3509	428	0.020
Total		17546167	1876339	100.000